

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012622\
 Data File : VW024447.D
 Acq On : 26 Jan 2022 18:20
 Operator : SY/MD
 Sample : N1275-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F51

Quant Time: Jan 27 03:52:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 01:56:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	154346	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	165841	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	80356	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	64868	4.797	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.000%
7) Chloroethane-d5	1.571	69	59538	5.048	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.000%
11) 1,1-Dichloroethene-d2	2.111	63	97477	3.771	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%
20) 2-Butanone-d5	3.896	46	125273	58.128	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.260%
24) Chloroform-d	4.352	84	130400	5.082	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
26) 1,2-Dichloroethane-d4	5.034	65	61021	5.251	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	5.053	84	242672	4.900	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
36) 1,2-Dichloropropane-d6	6.069	67	77961	4.998	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.000%
41) Toluene-d8	7.317	98	203613	4.480	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	7.625	79	24407	4.557	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.088	63	78180	42.691	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.380%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41123	4.430	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	77790	5.646	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.000%
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	10606	9.440	ug/L	68
25) Chloroform	4.375	83	2516	0.107	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024447.D
Acq On : 26 Jan 2022 18:20
Operator : SY/MD
Sample : N1275-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F51

Quant Time: Jan 27 03:52:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 01:56:16 2022
Response via : Initial Calibration




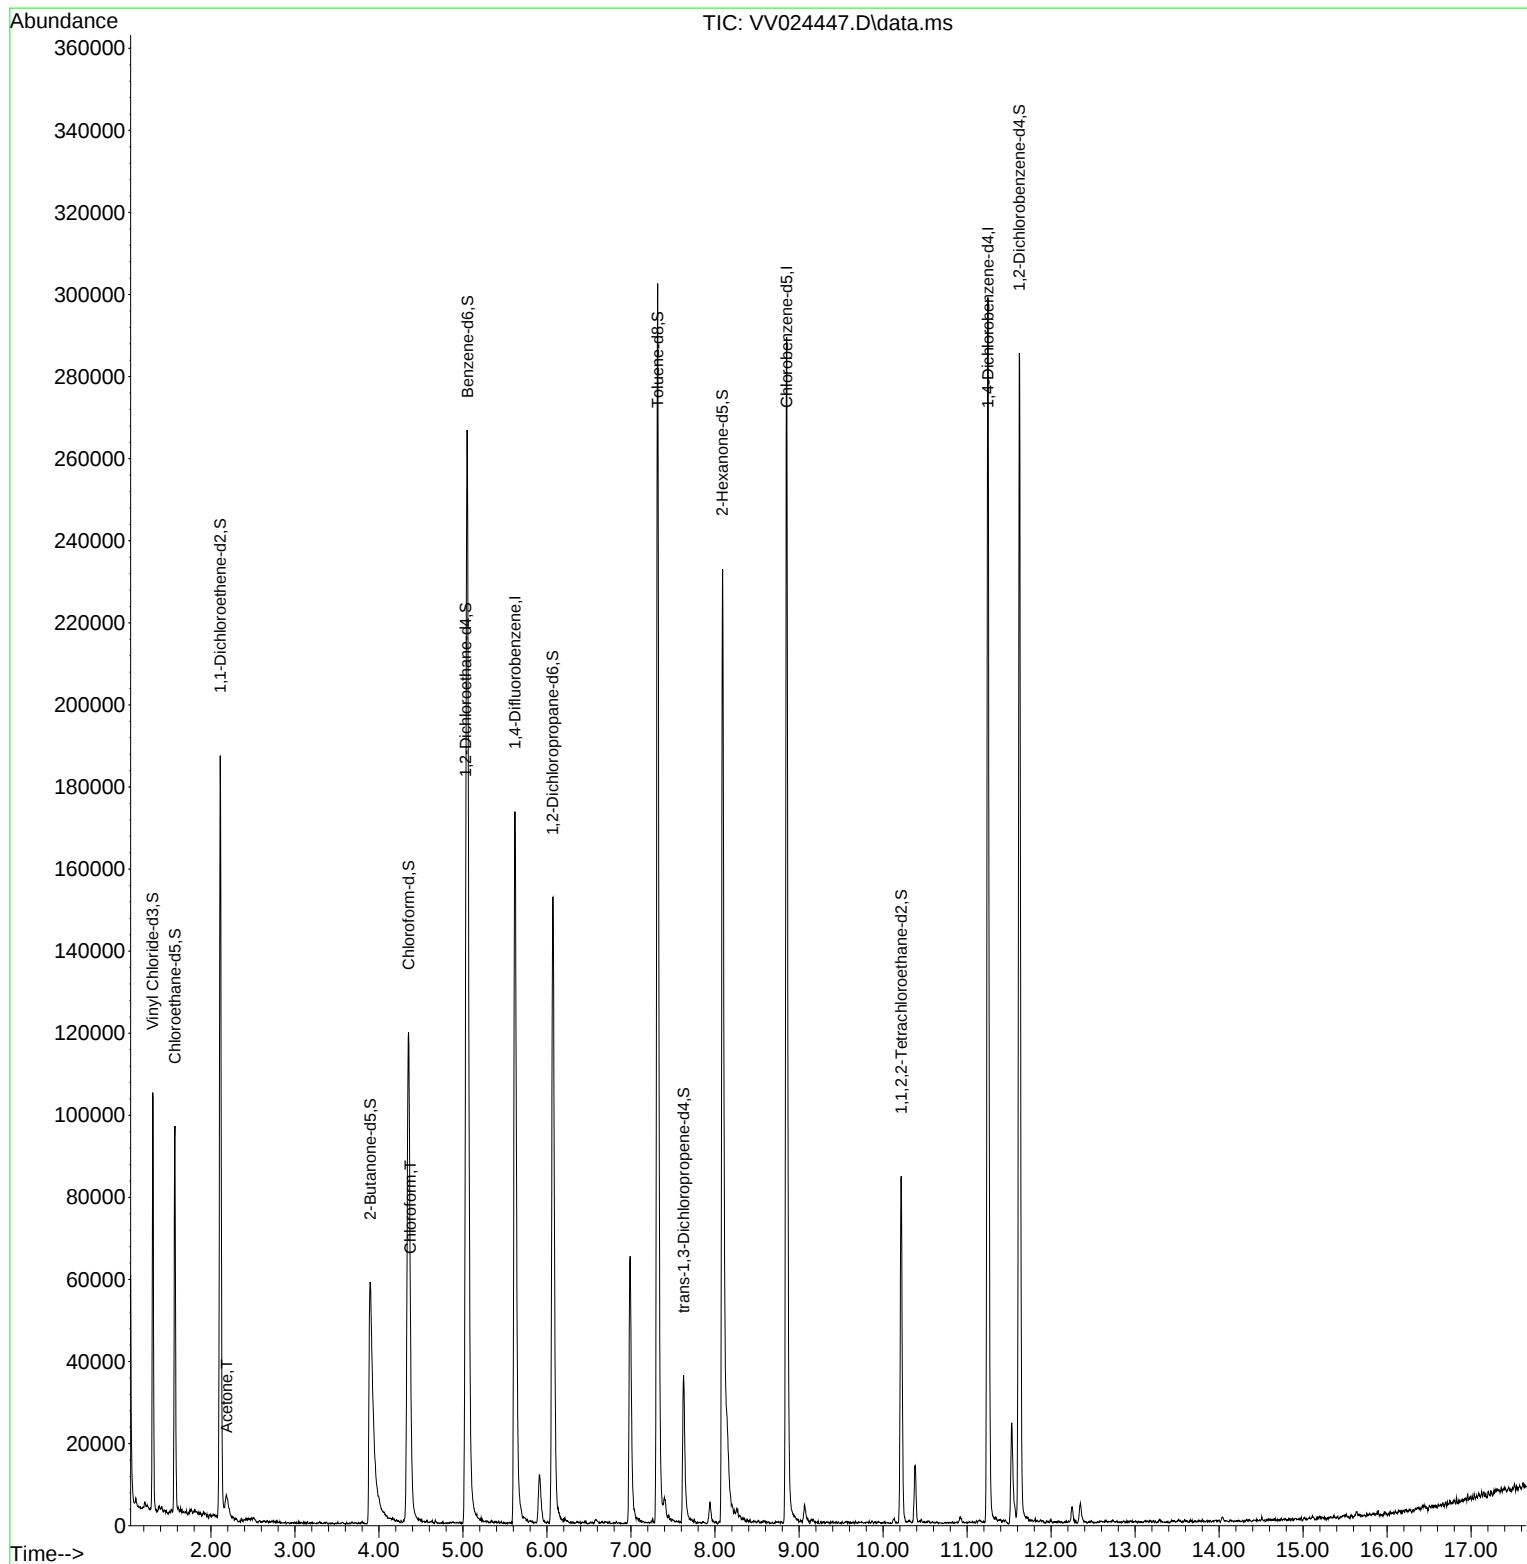


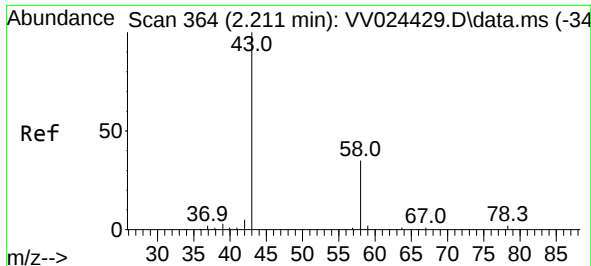

#13
Acetone
Concen: 9.440 ug/L
RT: 2.185 min Scan# 31
Delta R.T. -0.026 min
Lab File: VV024447.D
Acq: 26 Jan 2022 18:20

Instrument :
MSVOA_V
ClientSampleId :
C0F51

Tgt Ion: 43 Resp: 10606
Ion Ratio Lower Upper
43 100
58 35.7 0.0 41.4

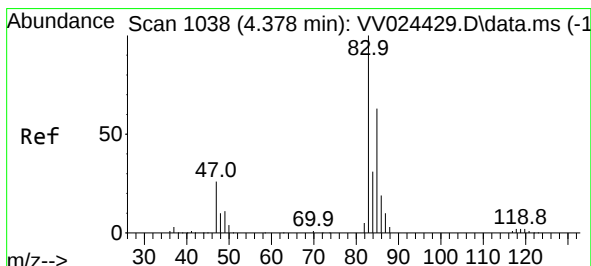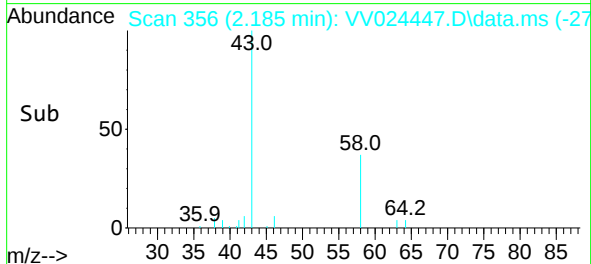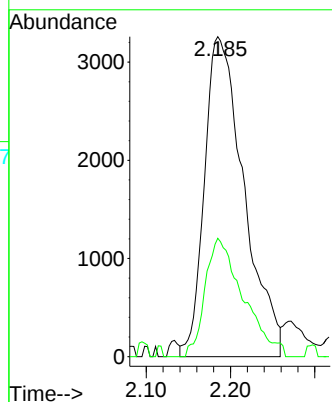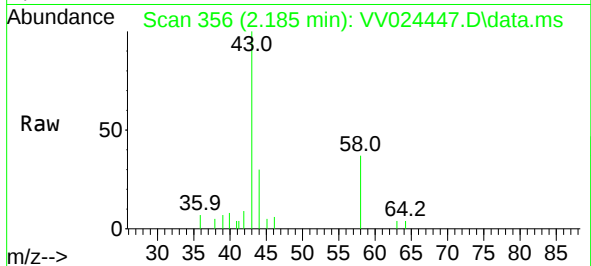

#25
Chloroform
Concen: 0.107 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. -0.003 min
Lab File: VV024447.D
Acq: 26 Jan 2022 18:20

Tgt Ion: 83 Resp: 2516
Ion Ratio Lower Upper
83 100
85 68.2 45.2 84.0

