

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012622\
 Data File : VW024448.D
 Acq On : 26 Jan 2022 18:43
 Operator : SY/MD
 Sample : N1275-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F52

Quant Time: Jan 27 03:52:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 01:56:16 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	154268	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	168171	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	82787	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	67886	5.023	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.400%		
7) Chloroethane-d5	1.571	69	63219	5.362	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 107.200%		
11) 1,1-Dichloroethene-d2	2.111	63	103484	4.006	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 80.200%		
20) 2-Butanone-d5	3.896	46	131701	61.142	ug/L	-0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	= 122.280%		
24) Chloroform-d	4.349	84	139674	5.446	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 109.000%		
26) 1,2-Dichloroethane-d4	5.034	65	65449	5.635	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 112.600%		
32) Benzene-d6	5.053	84	260819	5.193	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 103.800%		
36) 1,2-Dichloropropane-d6	6.069	67	83278	5.265	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 105.400%		
41) Toluene-d8	7.317	98	218112	4.733	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 94.600%		
43) trans-1,3-Dichloroprop...	7.625	79	24752	4.557	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 91.200%		
46) 2-Hexanone-d5	8.088	63	84399	45.449	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 90.900%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	42513	4.516	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 90.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	82966	5.844	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 116.800%		
Target Compounds						
13) Acetone	2.182	43	10095	8.990	ug/L	69
25) Chloroform	4.375	83	3131	0.133	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024448.D
Acq On : 26 Jan 2022 18:43
Operator : SY/MD
Sample : N1275-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F52

Quant Time: Jan 27 03:52:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 01:56:16 2022
Response via : Initial Calibration




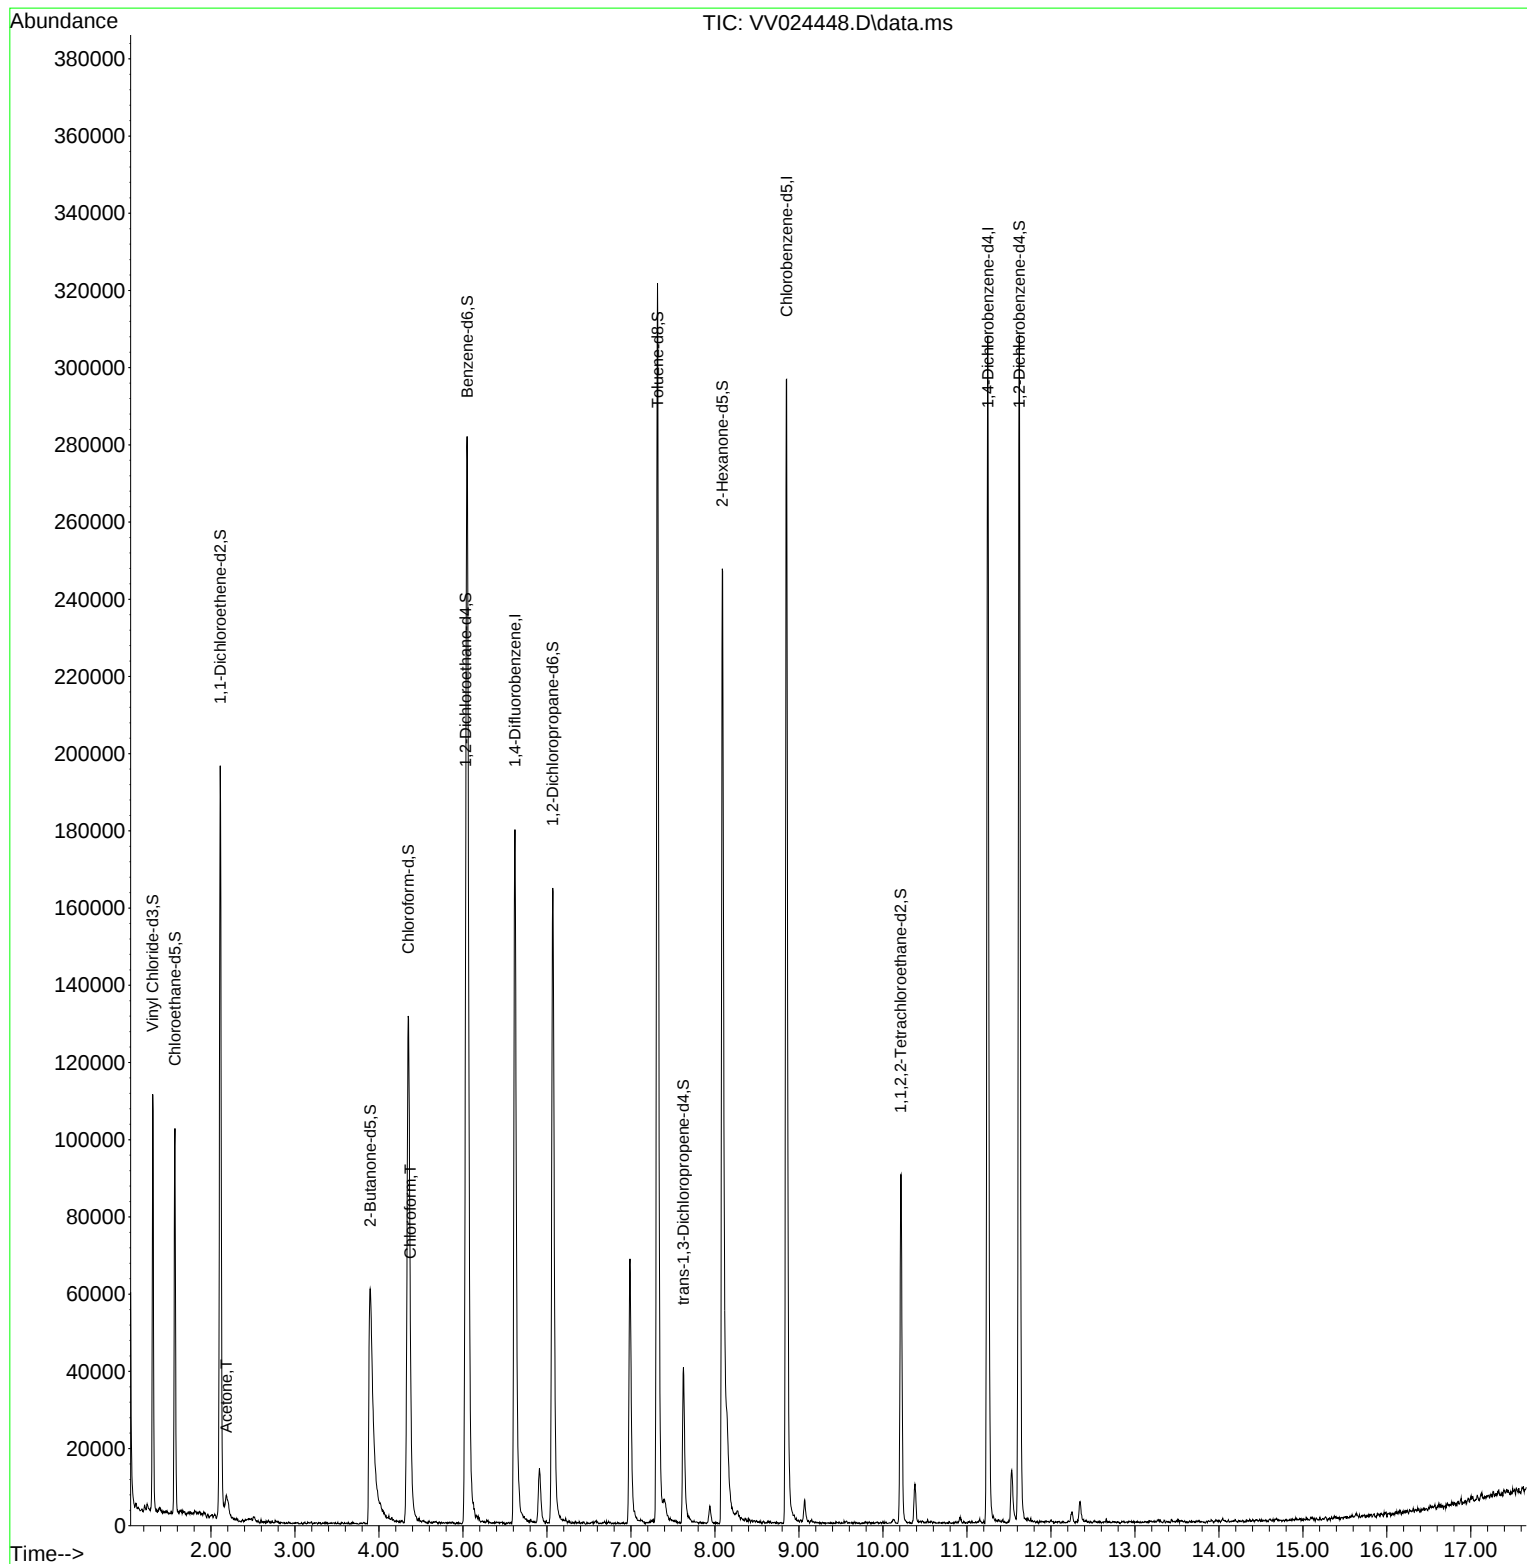


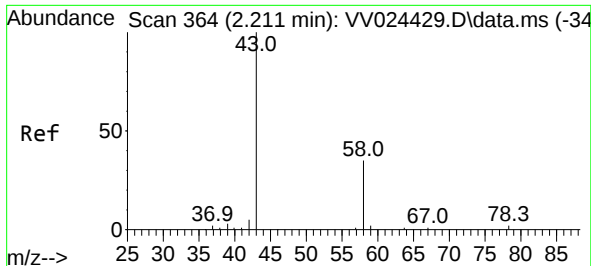

#13
Acetone
Concen: 8.990 ug/L
RT: 2.182 min Scan# 31
Delta R.T. -0.029 min
Lab File: VV024448.D
Acq: 26 Jan 2022 18:43

Instrument :
MSVOA_V
ClientSampleId :
C0F52

Tgt Ion: 43 Resp: 10095
Ion Ratio Lower Upper
43 100
58 35.0 0.0 41.4

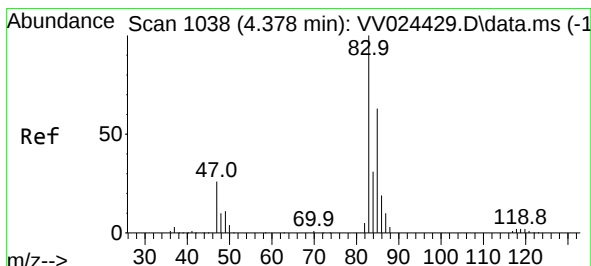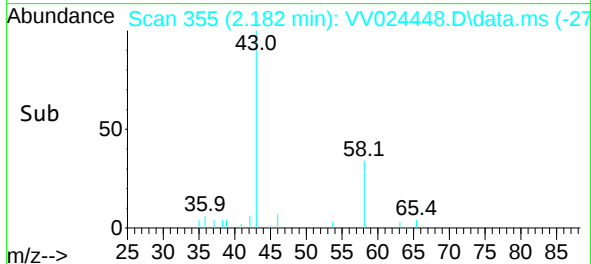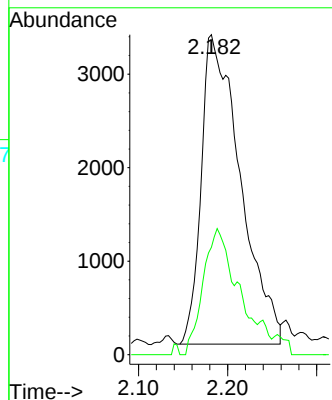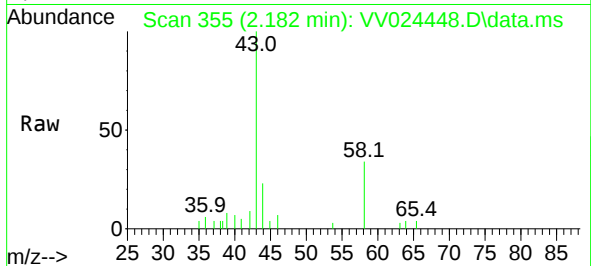

#25
Chloroform
Concen: 0.133 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. -0.003 min
Lab File: VV024448.D
Acq: 26 Jan 2022 18:43

Tgt Ion: 83 Resp: 3131
Ion Ratio Lower Upper
83 100
85 64.4 45.2 84.0

