

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024434.D
 Acq On : 26 Jan 2022 13:18
 Operator : SY/MD
 Sample : N1275-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024434.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	129575	128203	16.26%	2.158%
2	1.568	156	164	178	rVB	107655	124376	15.77%	2.093%
3	2.108	322	332	352	rVB	221042	324186	41.11%	5.456%
4	3.934	885	900	931	rBV2	26997	147421	18.69%	2.481%
5	4.349	1014	1029	1060	rVB2	138226	358150	45.41%	6.027%
6	5.050	1231	1247	1276	rBV2	311556	788664	100.00%	13.273%
7	5.619	1413	1424	1446	rBV	188214	390927	49.57%	6.579%
8	5.908	1502	1514	1515	rBV6	9240	9792	1.24%	0.165%
9	6.069	1545	1564	1593	rBV	177537	378851	48.04%	6.376%
10	6.989	1837	1850	1875	rBV	78083	153910	19.52%	2.590%
11	7.317	1939	1952	1971	rBV	360973	642724	81.50%	10.817%
12	7.625	2036	2048	2073	rBV2	44673	88570	11.23%	1.491%
13	7.937	2134	2145	2152	rBV4	6113	10224	1.30%	0.172%
14	8.095	2181	2194	2238	rBV	213026	592587	75.14%	9.973%
15	8.850	2416	2429	2451	rBV	316496	530538	67.27%	8.929%
16	9.072	2487	2498	2512	rVB3	5254	10418	1.32%	0.175%
17	10.217	2842	2854	2871	rBV	104749	174530	22.13%	2.937%
18	10.384	2896	2906	2915	rVB3	7456	12186	1.55%	0.205%
19	11.249	3164	3175	3196	rBV	335191	528371	67.00%	8.892%
20	11.622	3280	3291	3318	rBV	333343	547428	69.41%	9.213%




Sum of corrected areas: 5942056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024434.D
Acq On : 26 Jan 2022 13:18
Operator : SY/MD
Sample : N1275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

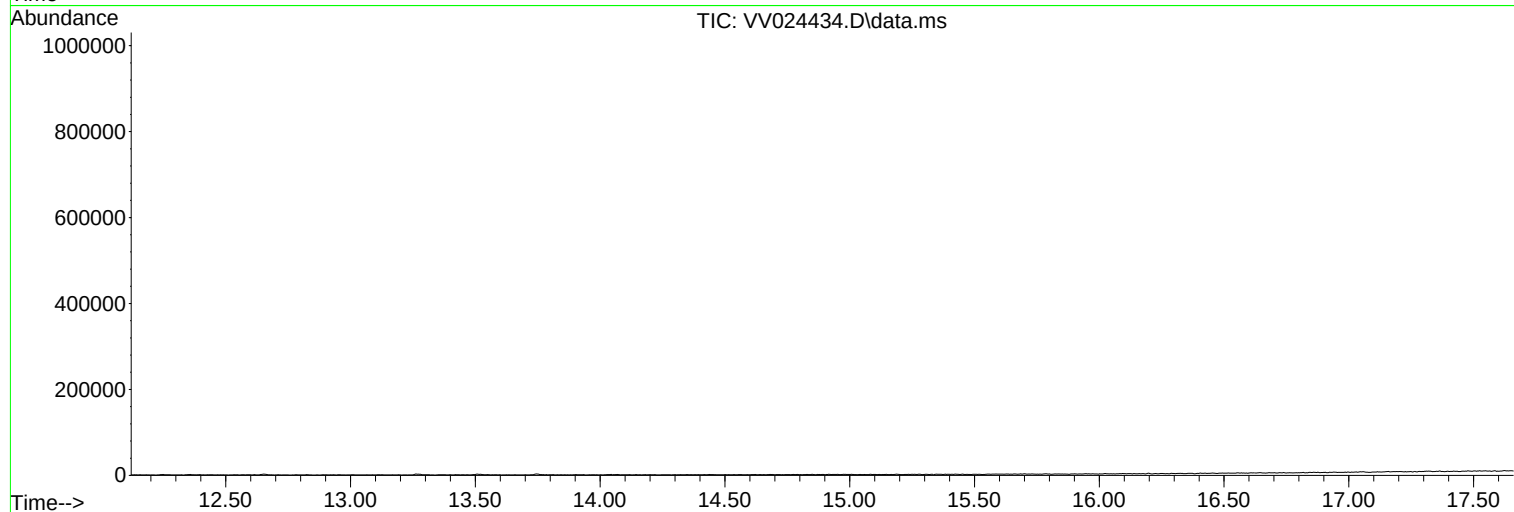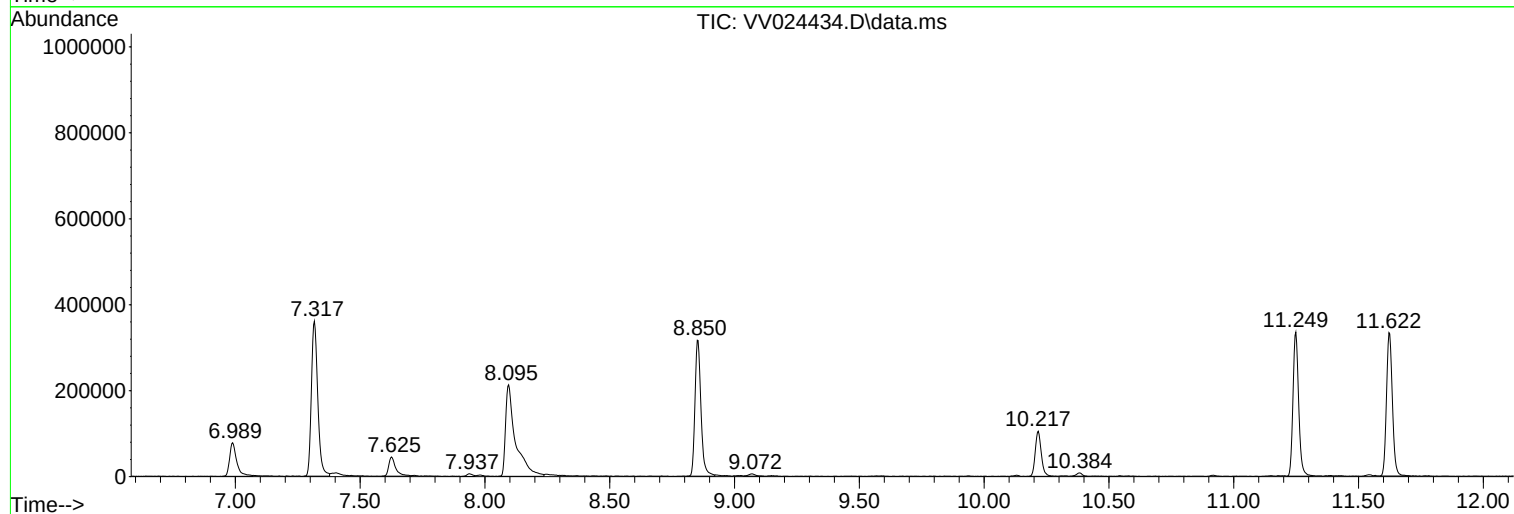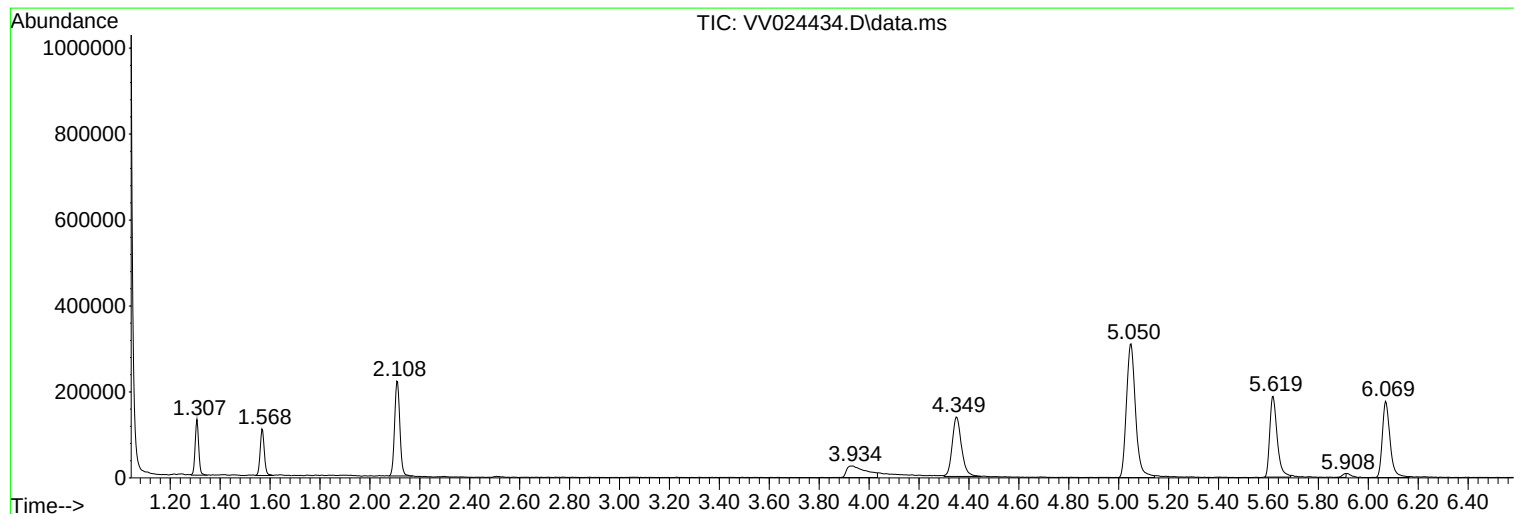

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024434.D
Acq On : 26 Jan 2022 13:18
Operator : SY/MD
Sample : N1275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024434.D
Acq On : 26 Jan 2022 13:18
Operator : SY/MD
Sample : N1275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------