

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024435.D
 Acq On : 26 Jan 2022 13:41
 Operator : SY/MD
 Sample : N1275-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F24

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	121058	120052	16.61%	2.111%
2	1.568	156	164	179	rVB	106683	121838	16.85%	2.143%
3	2.108	322	332	350	rVB	206440	305571	42.27%	5.374%
4	3.921	885	896	925	rBV	27687	130472	18.05%	2.294%
5	4.352	1013	1030	1055	rVB	130051	336277	46.52%	5.914%
6	5.050	1229	1247	1276	rBV2	285419	722867	100.00%	12.712%
7	5.619	1413	1424	1447	rBV	193870	399783	55.31%	7.031%
8	5.911	1505	1515	1530	rBV7	8392	18941	2.62%	0.333%
9	6.069	1546	1564	1595	rBV2	164770	353050	48.84%	6.209%
10	6.989	1840	1850	1868	rBV	71582	138339	19.14%	2.433%
11	7.317	1941	1952	1971	rBV	335903	583073	80.66%	10.254%
12	7.625	2038	2048	2074	rBV	41510	81724	11.31%	1.437%
13	7.937	2137	2145	2156	rBV4	8884	16121	2.23%	0.284%
14	8.091	2182	2193	2236	rBV	206297	553986	76.64%	9.742%
15	8.853	2418	2430	2449	rBV	316947	531741	73.56%	9.351%
16	10.217	2839	2854	2872	rBV	99002	164925	22.82%	2.900%
17	10.381	2894	2905	2919	rVB2	17864	30287	4.19%	0.533%
18	11.249	3163	3175	3191	rBV	329675	524233	72.52%	9.219%
19	11.535	3254	3264	3279	rBV3	23937	47255	6.54%	0.831%
20	11.625	3280	3292	3309	rVB	316286	505824	69.97%	8.895%




Sum of corrected areas: 5686359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024435.D
Acq On : 26 Jan 2022 13:41
Operator : SY/MD
Sample : N1275-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

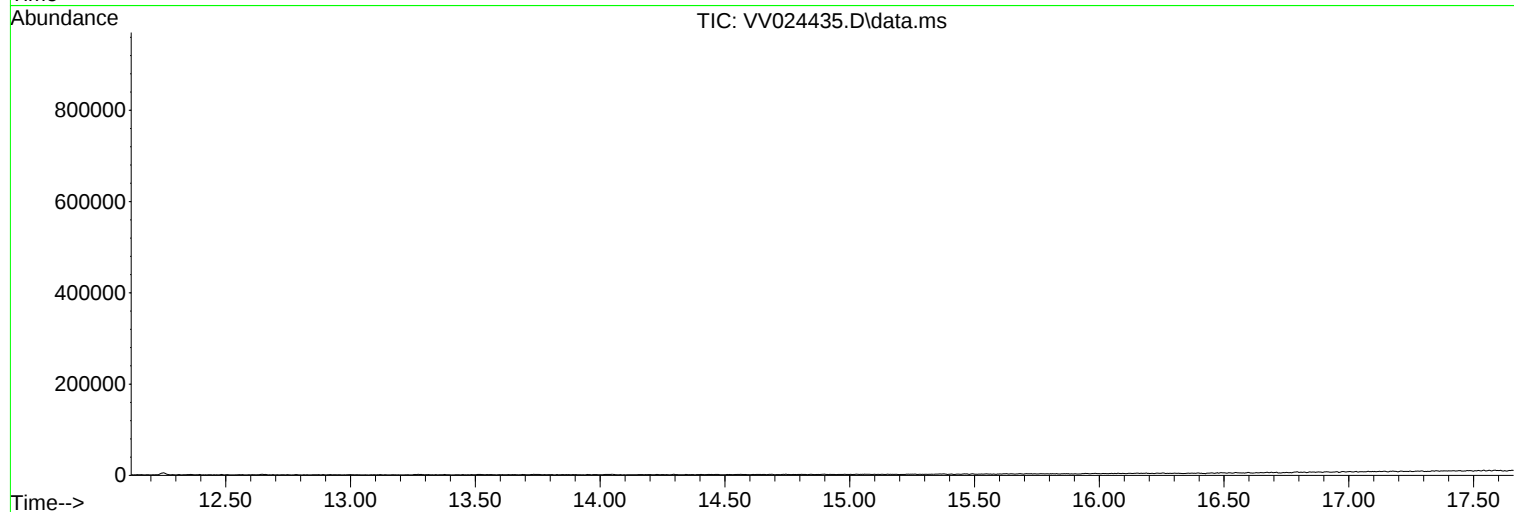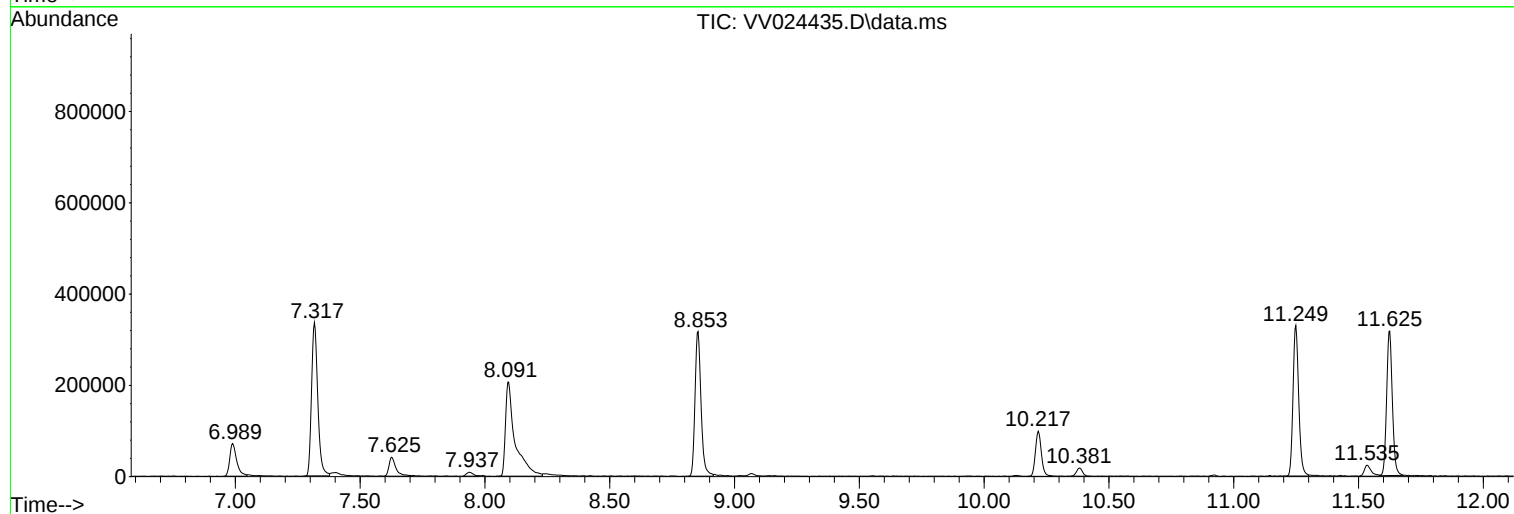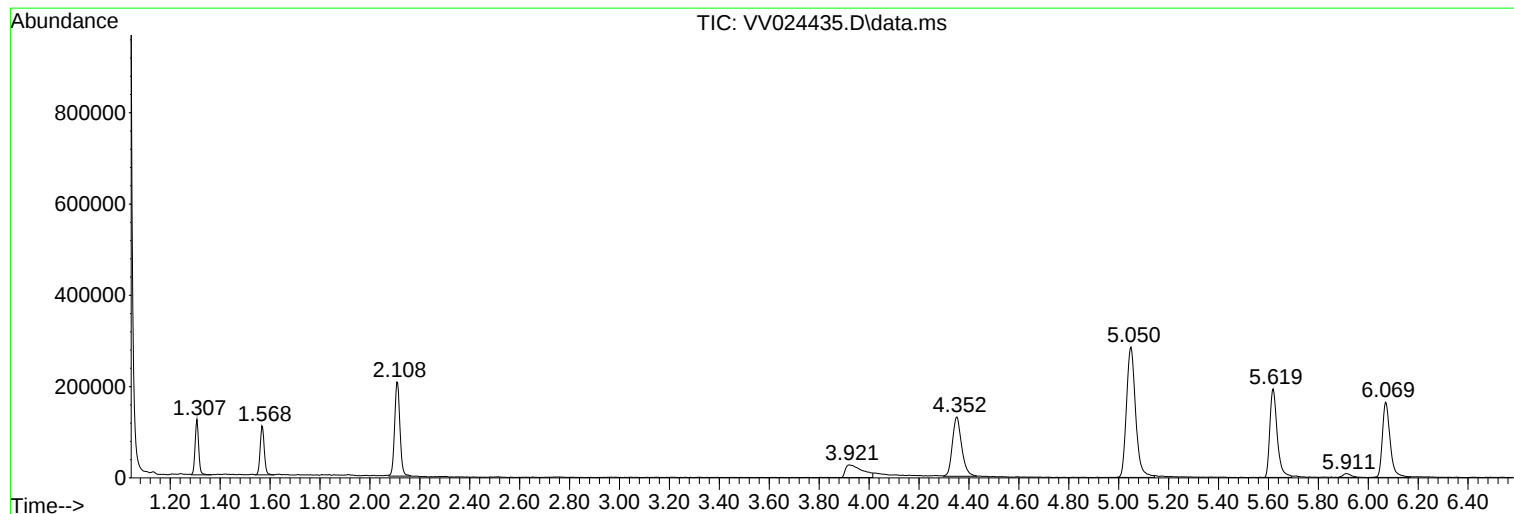

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024435.D
Acq On : 26 Jan 2022 13:41
Operator : SY/MD
Sample : N1275-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024435.D
Acq On : 26 Jan 2022 13:41
Operator : SY/MD
Sample : N1275-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
