

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024436.D
 Acq On : 26 Jan 2022 14:04
 Operator : SY/MD
 Sample : N1275-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F25

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rBV	124497	119721	16.50%	2.116%
2	1.568	156	164	178	rBV	109328	121831	16.79%	2.153%
3	2.108	322	332	353	rVB	211448	312833	43.11%	5.529%
4	3.915	881	894	921	rBV	31589	139900	19.28%	2.473%
5	4.349	1014	1029	1055	rVB2	131396	351651	48.45%	6.215%
6	5.047	1230	1246	1275	rBV2	288150	725738	100.00%	12.826%
7	5.616	1408	1423	1447	rBV	184934	391200	53.90%	6.914%
8	5.915	1505	1516	1531	rBV7	13288	34572	4.76%	0.611%
9	6.069	1551	1564	1587	rBV	165006	353401	48.70%	6.246%
10	6.989	1838	1850	1871	rBV	72128	143135	19.72%	2.530%
11	7.317	1941	1952	1971	rBV	329887	583842	80.45%	10.319%
12	7.625	2037	2048	2065	rBV2	41933	79985	11.02%	1.414%
13	7.937	2133	2145	2154	rBV2	8249	16023	2.21%	0.283%
14	8.092	2183	2193	2239	rBV	211250	564082	77.73%	9.969%
15	8.850	2417	2429	2453	rBV	306228	516808	71.21%	9.134%
16	10.217	2842	2854	2875	rBV	98350	166268	22.91%	2.939%
17	10.381	2894	2905	2918	rVB	17268	26911	3.71%	0.476%
18	11.249	3163	3175	3191	rBV	317060	501626	69.12%	8.866%
19	11.535	3255	3264	3273	rBV3	12793	23023	3.17%	0.407%
20	11.622	3281	3291	3309	rBV	305942	485598	66.91%	8.582%




Sum of corrected areas: 5658148

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024436.D
Acq On : 26 Jan 2022 14:04
Operator : SY/MD
Sample : N1275-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

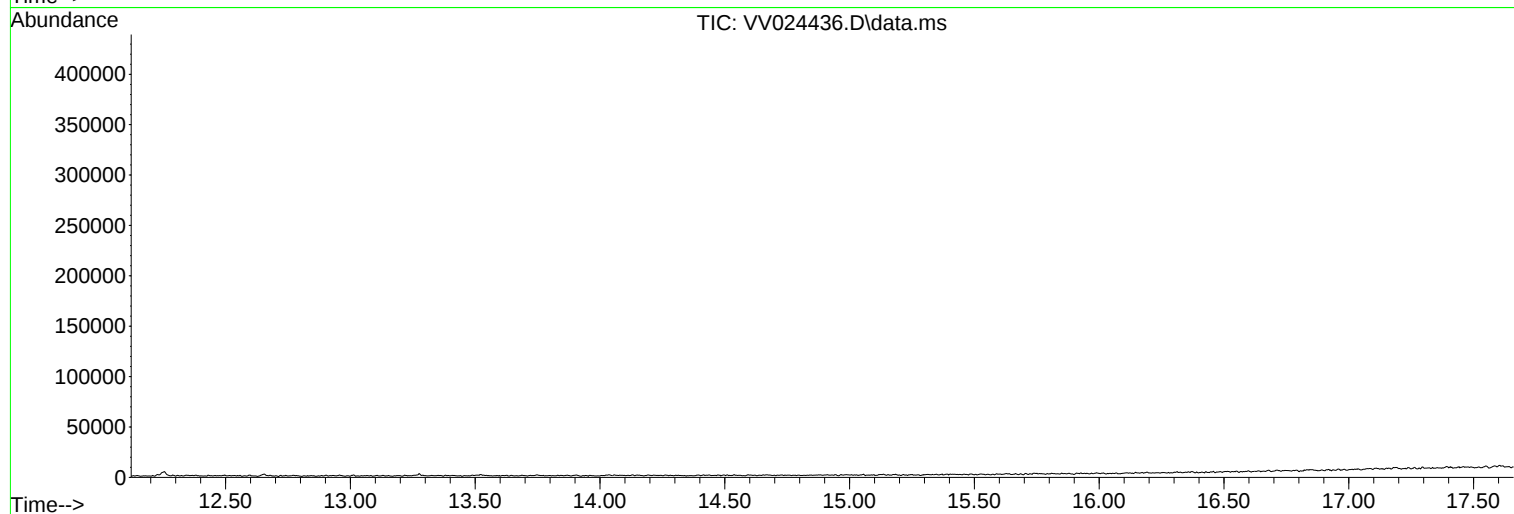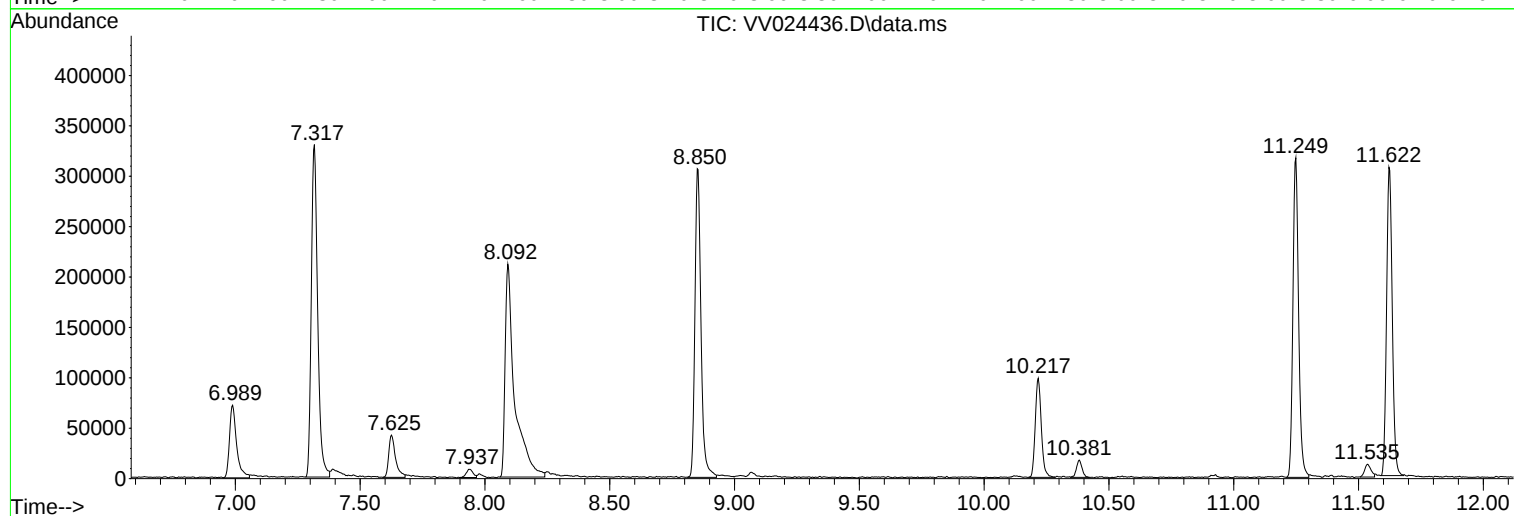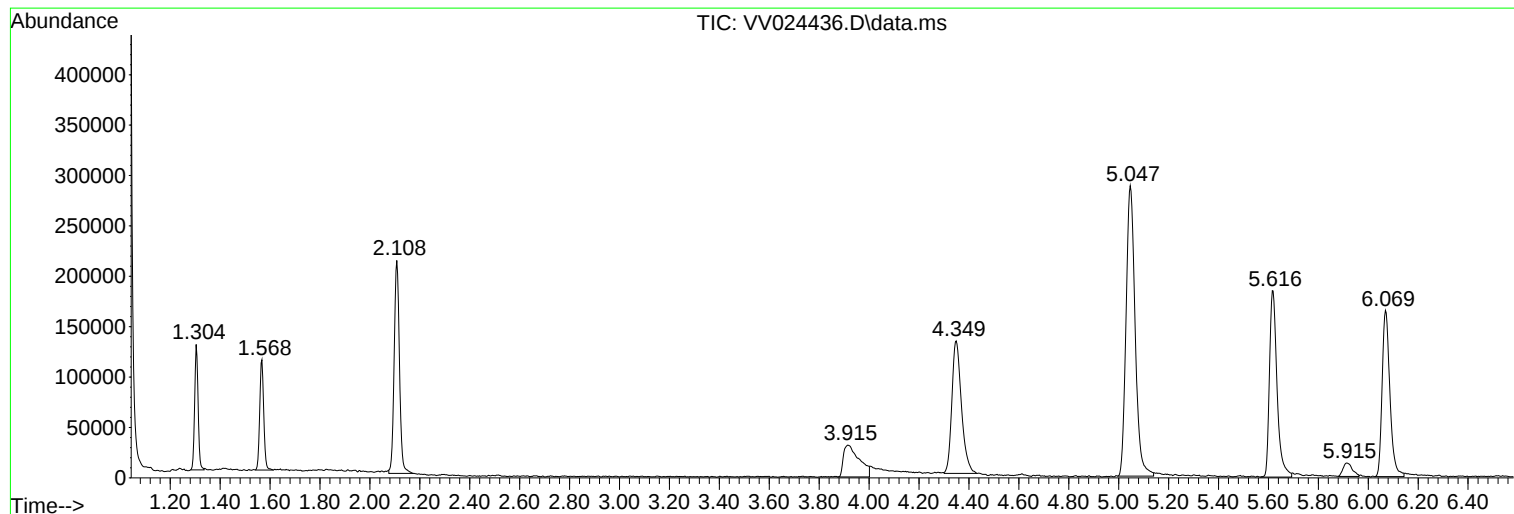

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024436.D
Acq On : 26 Jan 2022 14:04
Operator : SY/MD
Sample : N1275-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024436.D
Acq On : 26 Jan 2022 14:04
Operator : SY/MD
Sample : N1275-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc