

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024438.D
 Acq On : 26 Jan 2022 14:51
 Operator : SY/MD
 Sample : N1275-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	114574	119756	16.73%	2.144%
2	1.571	156	165	177	rBV	110745	126263	17.63%	2.261%
3	2.111	321	333	352	rVB	208684	305694	42.69%	5.474%
4	3.915	883	894	918	rBV2	43043	180255	25.17%	3.227%
5	4.352	1013	1030	1051	rBV	127280	334947	46.78%	5.997%
6	5.050	1231	1247	1269	rBV3	284880	716021	100.00%	12.820%
7	5.619	1412	1424	1452	rBV	181278	383027	53.49%	6.858%
8	5.915	1504	1516	1528	rBV	9488	25163	3.51%	0.451%
9	6.069	1551	1564	1589	rBV	167398	358952	50.13%	6.427%
10	6.989	1840	1850	1877	rBV	70278	137835	19.25%	2.468%
11	7.317	1940	1952	1971	rBV	315244	566377	79.10%	10.141%
12	7.625	2036	2048	2063	rBV2	41076	79174	11.06%	1.418%
13	7.934	2137	2144	2153	rBV2	5244	9786	1.37%	0.175%
14	8.091	2182	2193	2226	rBV	253563	553699	77.33%	9.914%
15	8.850	2419	2429	2452	rBV	306786	510927	71.36%	9.148%
16	9.072	2489	2498	2506	rVB5	4974	8895	1.24%	0.159%
17	10.217	2842	2854	2867	rBV	98178	161372	22.54%	2.889%
18	10.381	2896	2905	2916	rVB5	11211	19432	2.71%	0.348%
19	11.249	3164	3175	3193	rBV	307506	487922	68.14%	8.736%
20	11.535	3253	3264	3273	rBV2	16678	31365	4.38%	0.562%
21	11.622	3280	3291	3309	rBV	294241	468113	65.38%	8.382%




Sum of corrected areas: 5584975

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024438.D
Acq On : 26 Jan 2022 14:51
Operator : SY/MD
Sample : N1275-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

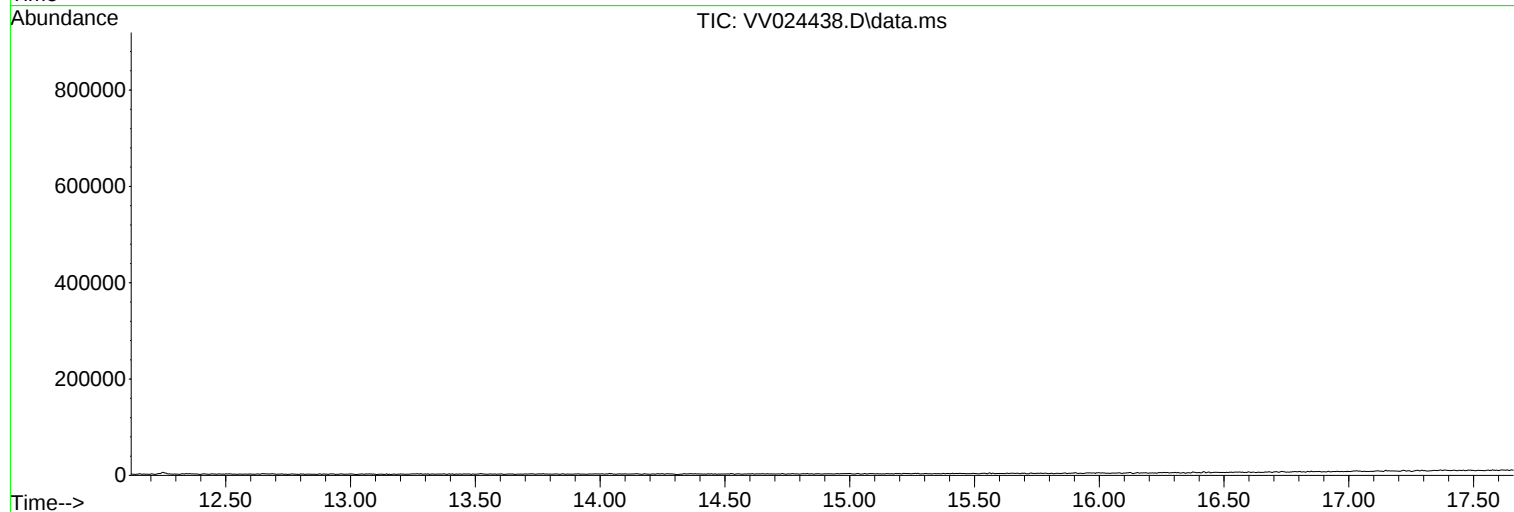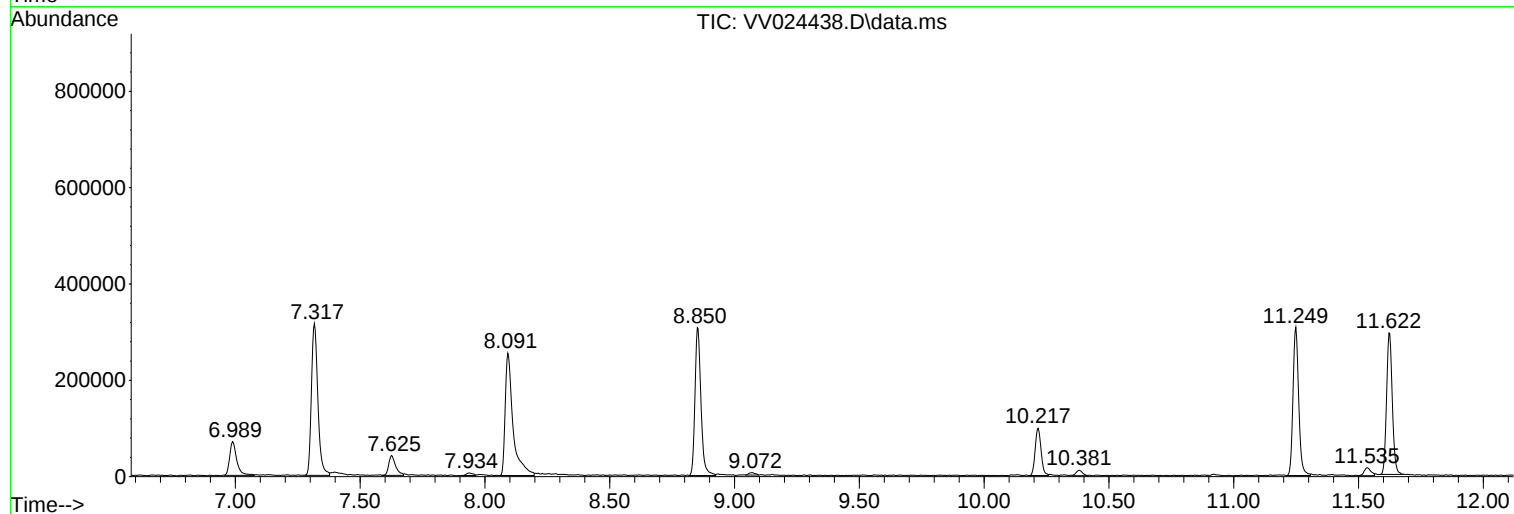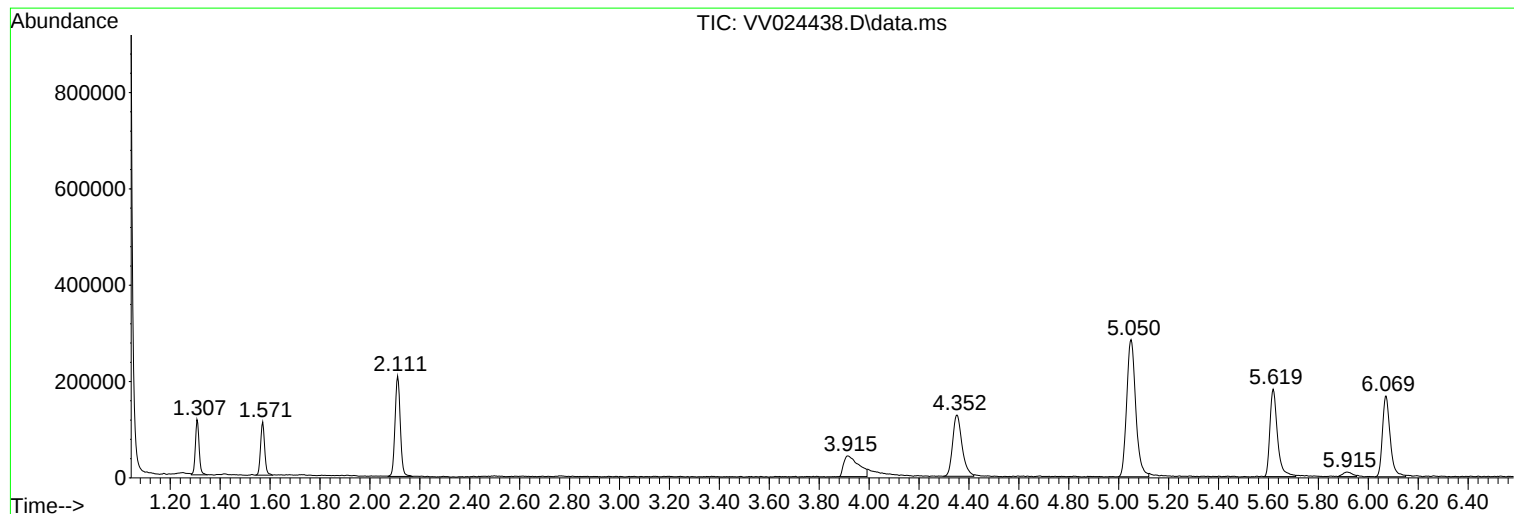

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024438.D
Acq On : 26 Jan 2022 14:51
Operator : SY/MD
Sample : N1275-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024438.D
Acq On : 26 Jan 2022 14:51
Operator : SY/MD
Sample : N1275-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc