

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024439.D
 Acq On : 26 Jan 2022 15:14
 Operator : SY/MD
 Sample : N1275-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	117915	122311	16.65%	2.242%
2	1.568	157	164	174	rBV	105231	119319	16.24%	2.187%
3	2.111	322	333	351	rVB	206961	304049	41.39%	5.573%
4	3.915	883	894	915	rBV2	34765	132138	17.99%	2.422%
5	4.349	1014	1029	1052	rVB	127324	324121	44.13%	5.941%
6	5.050	1230	1247	1283	rBV2	285104	734519	100.00%	13.464%
7	5.619	1412	1424	1449	rBV	171607	363417	49.48%	6.662%
8	5.908	1505	1514	1515	rBV7	10849	10799	1.47%	0.198%
9	6.069	1552	1564	1587	rBV	169962	360932	49.14%	6.616%
10	6.989	1840	1850	1869	rBV	70300	136099	18.53%	2.495%
11	7.317	1939	1952	1972	rBV	319408	570733	77.70%	10.462%
12	7.625	2040	2048	2067	rBV2	41608	77680	10.58%	1.424%
13	8.092	2181	2193	2230	rBV	221236	566455	77.12%	10.383%
14	8.854	2419	2430	2454	rBV	292391	487965	66.43%	8.945%
15	10.217	2843	2854	2871	rBV	98653	165485	22.53%	3.033%
16	10.381	2896	2905	2913	rBV2	8713	13273	1.81%	0.243%
17	11.249	3164	3175	3191	rBV	292849	460961	62.76%	8.450%
18	11.535	3255	3264	3277	rBV3	12977	25936	3.53%	0.475%
19	11.622	3280	3291	3311	rVV	298744	479244	65.25%	8.785%




Sum of corrected areas: 5455436

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024439.D
Acq On : 26 Jan 2022 15:14
Operator : SY/MD
Sample : N1275-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

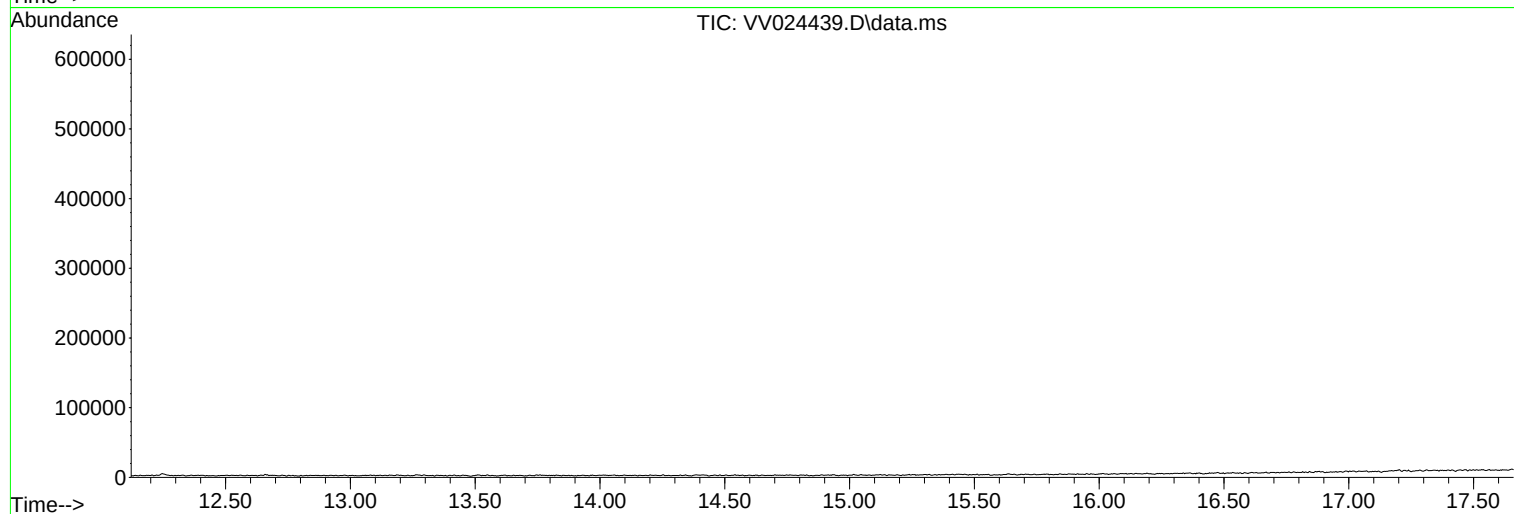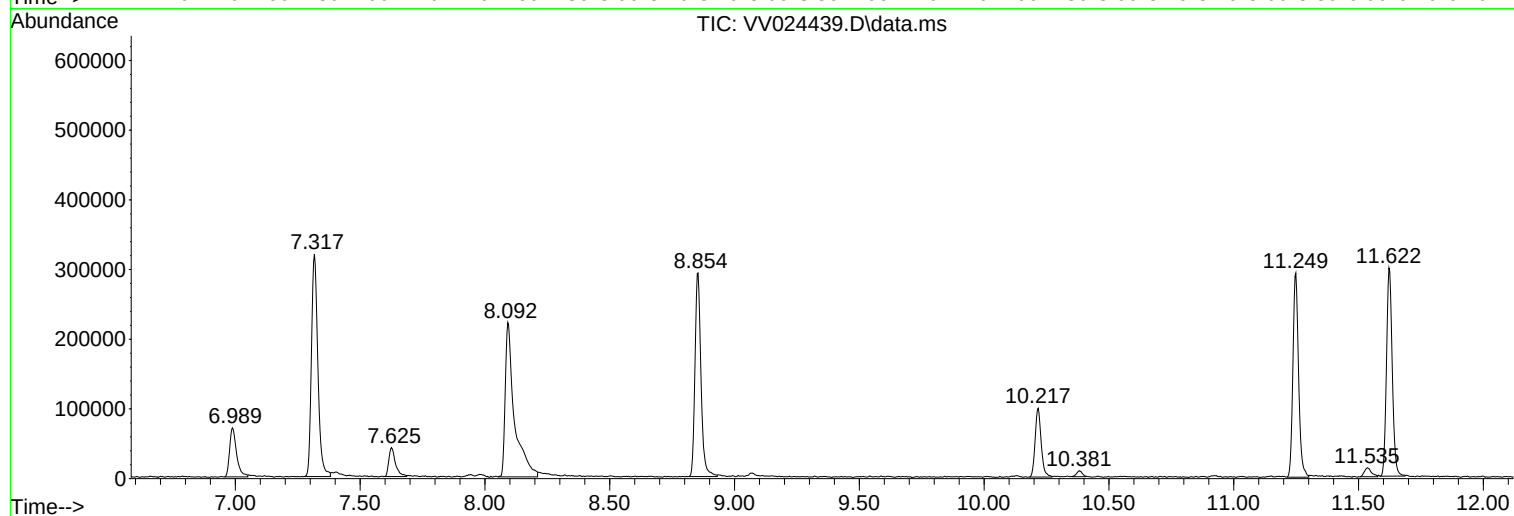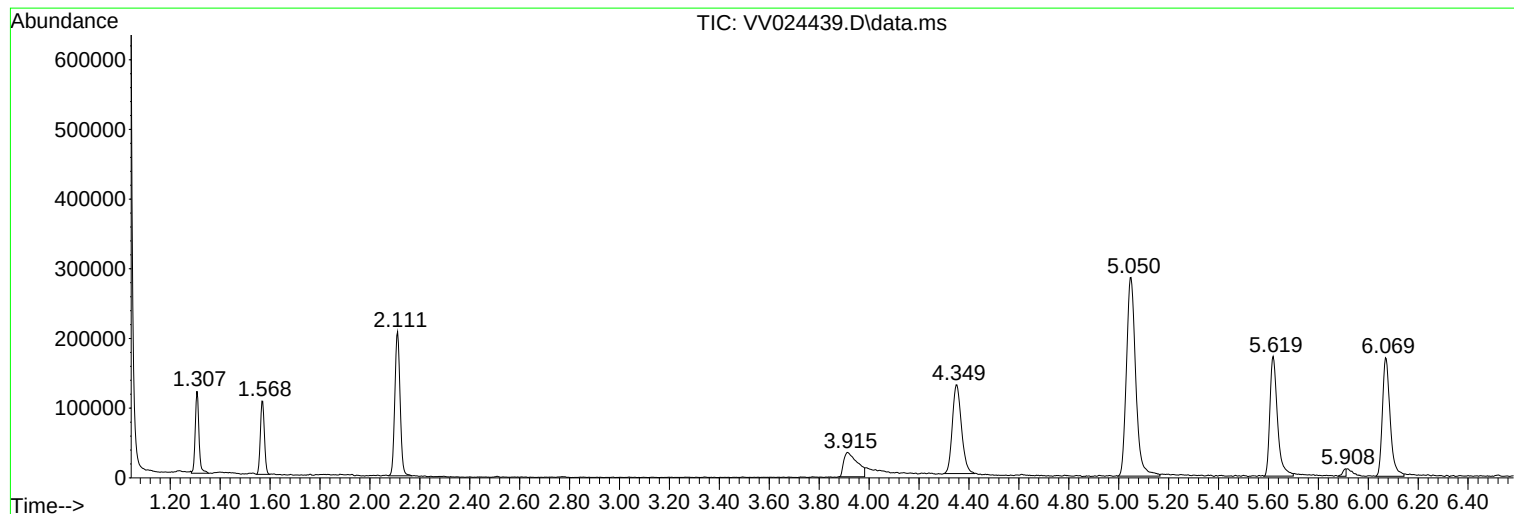

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024439.D
Acq On : 26 Jan 2022 15:14
Operator : SY/MD
Sample : N1275-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024439.D
Acq On : 26 Jan 2022 15:14
Operator : SY/MD
Sample : N1275-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------