

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024445.D
 Acq On : 26 Jan 2022 17:33
 Operator : SY/MD
 Sample : N1275-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F47

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	112316	110197	15.71%	2.032%
2	1.568	157	164	177	rVB	100867	113857	16.23%	2.099%
3	2.111	321	333	351	rVB	195620	289223	41.23%	5.333%
4	3.908	882	892	916	rBV2	38705	147402	21.01%	2.718%
5	4.352	1013	1030	1059	rBV2	125841	334960	47.75%	6.176%
6	5.050	1231	1247	1272	rBV2	281630	701554	100.00%	12.935%
7	5.619	1411	1424	1448	rBV	175788	368218	52.49%	6.789%
8	5.918	1504	1517	1534	rBV8	17675	42769	6.10%	0.789%
9	6.069	1550	1564	1584	rBV	160079	336132	47.91%	6.198%
10	6.989	1839	1850	1875	rBV	66328	130378	18.58%	2.404%
11	7.317	1941	1952	1972	rBV	313013	557379	79.45%	10.277%
12	7.625	2037	2048	2074	rBV	39964	78180	11.14%	1.442%
13	7.940	2134	2146	2153	rBV3	4597	9442	1.35%	0.174%
14	8.091	2183	2193	2226	rBV	225930	523678	74.65%	9.656%
15	8.854	2418	2430	2453	rBV	300067	498547	71.06%	9.192%
16	10.217	2842	2854	2870	rBV2	98990	159609	22.75%	2.943%
17	10.381	2896	2905	2916	rVB	10333	17414	2.48%	0.321%
18	11.249	3162	3175	3203	rBV	308437	488983	69.70%	9.016%
19	11.532	3253	3263	3279	rBV3	15067	30038	4.28%	0.554%
20	11.625	3279	3292	3314	rVB	303982	485520	69.21%	8.952%




Sum of corrected areas: 5423480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024445.D
Acq On : 26 Jan 2022 17:33
Operator : SY/MD
Sample : N1275-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

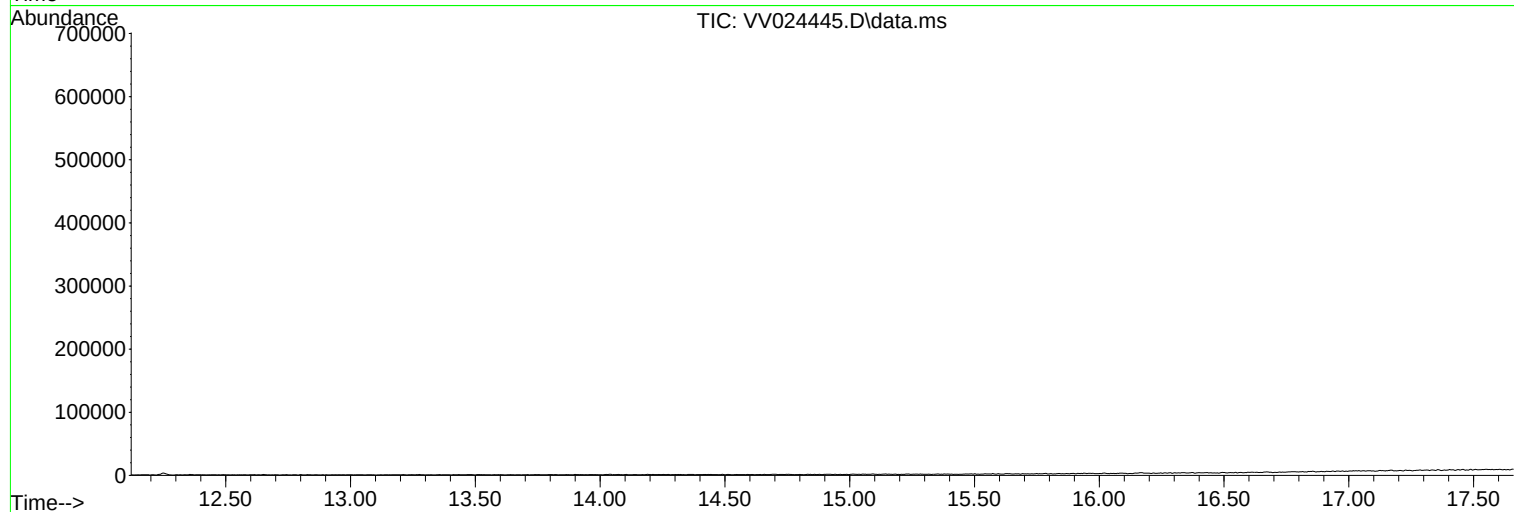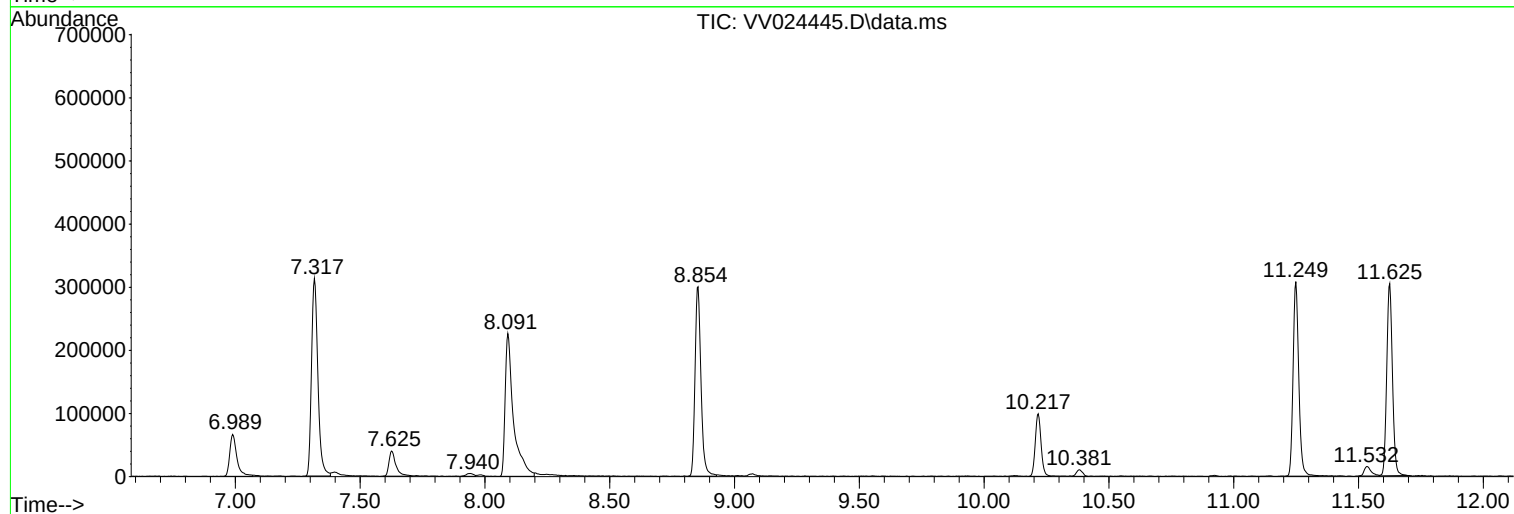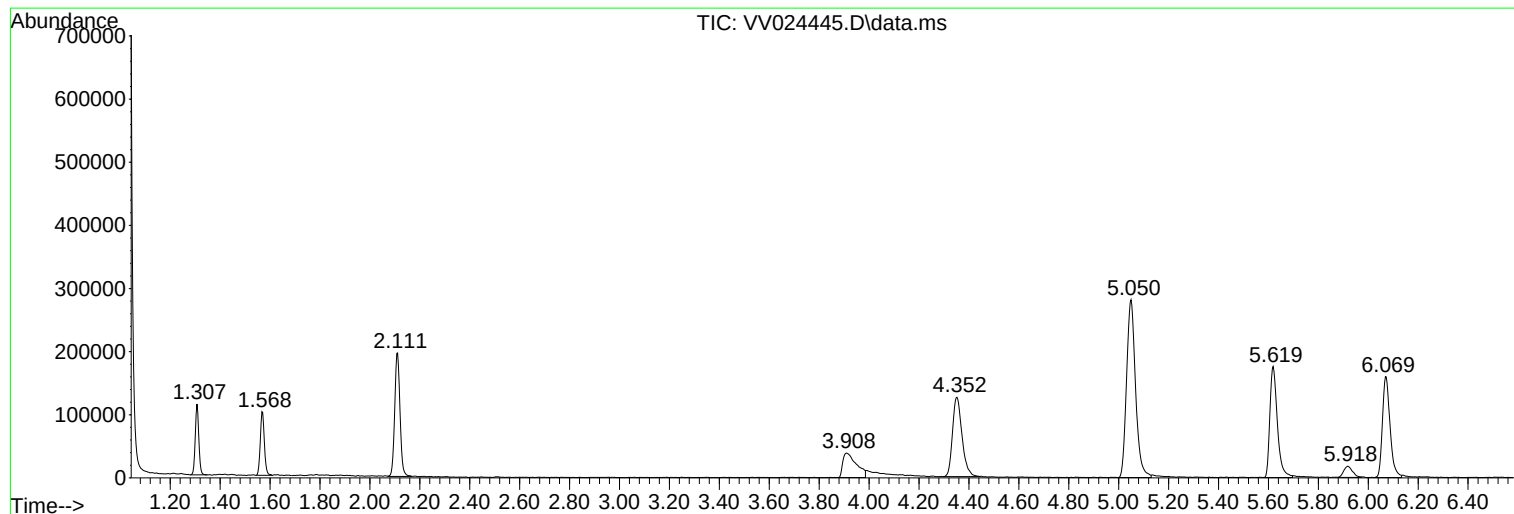

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024445.D
Acq On : 26 Jan 2022 17:33
Operator : SY/MD
Sample : N1275-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024445.D
Acq On : 26 Jan 2022 17:33
Operator : SY/MD
Sample : N1275-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------