

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024449.D
 Acq On : 26 Jan 2022 19:06
 Operator : SY/MD
 Sample : N1275-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	106297	108978	15.27%	1.975%
2	1.571	156	165	177	rBV	101328	113911	15.97%	2.064%
3	2.111	322	333	348	rBV	194394	282073	39.54%	5.111%
4	3.902	880	890	924	rBV	52882	218056	30.56%	3.951%
5	4.352	1012	1030	1056	rBV	131112	351767	49.31%	6.374%
6	5.050	1230	1247	1276	rBV2	282641	713444	100.00%	12.927%
7	5.619	1410	1424	1449	rBV	173268	366712	51.40%	6.645%
8	5.912	1502	1515	1531	rBV8	11941	29050	4.07%	0.526%
9	6.069	1551	1564	1592	rBV	162943	342594	48.02%	6.208%
10	6.989	1838	1850	1873	rBV	67457	132691	18.60%	2.404%
11	7.317	1940	1952	1972	rBV	317015	563705	79.01%	10.214%
12	7.625	2037	2048	2069	rBV	41158	75742	10.62%	1.372%
13	8.092	2183	2193	2226	rBV	259733	535540	75.06%	9.704%
14	8.854	2418	2430	2453	rBV	298258	497274	69.70%	9.010%
15	9.069	2487	2497	2505	rBV3	5267	8469	1.19%	0.153%
16	10.217	2841	2854	2867	rBV	98761	159842	22.40%	2.896%
17	10.381	2895	2905	2918	rVB2	10073	16470	2.31%	0.298%
18	11.249	3163	3175	3203	rBV	307682	484010	67.84%	8.770%
19	11.535	3254	3264	3277	rBV3	15289	28071	3.93%	0.509%
20	11.622	3279	3291	3311	rVV	311584	490602	68.77%	8.889%




Sum of corrected areas: 5519001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024449.D
Acq On : 26 Jan 2022 19:06
Operator : SY/MD
Sample : N1275-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

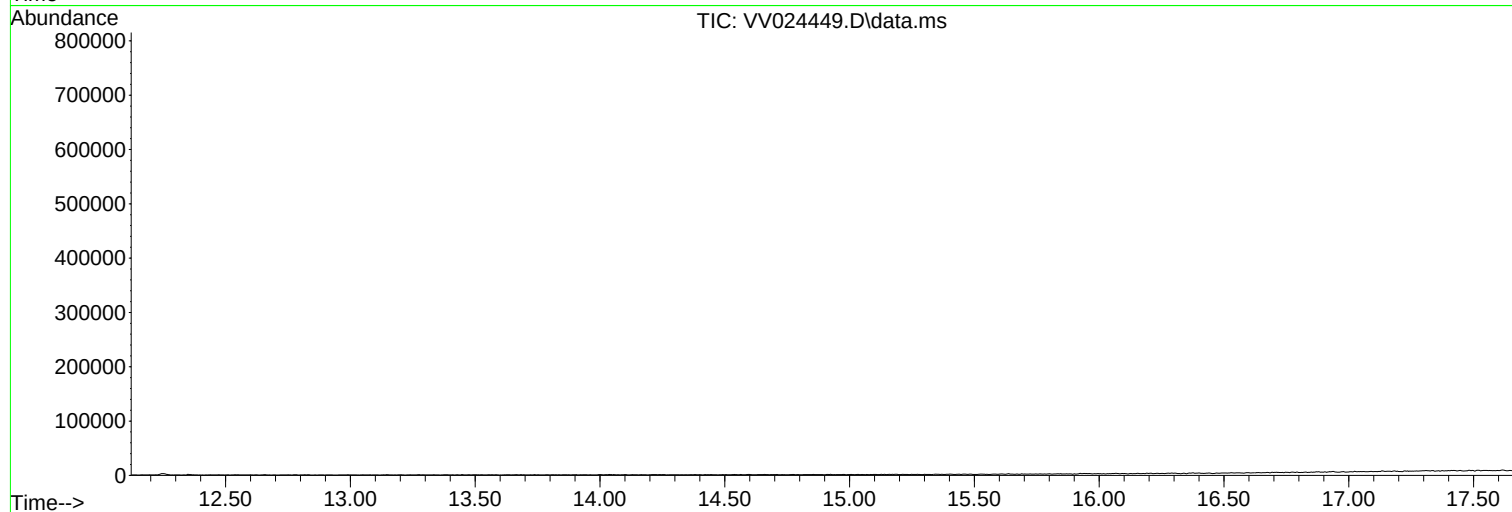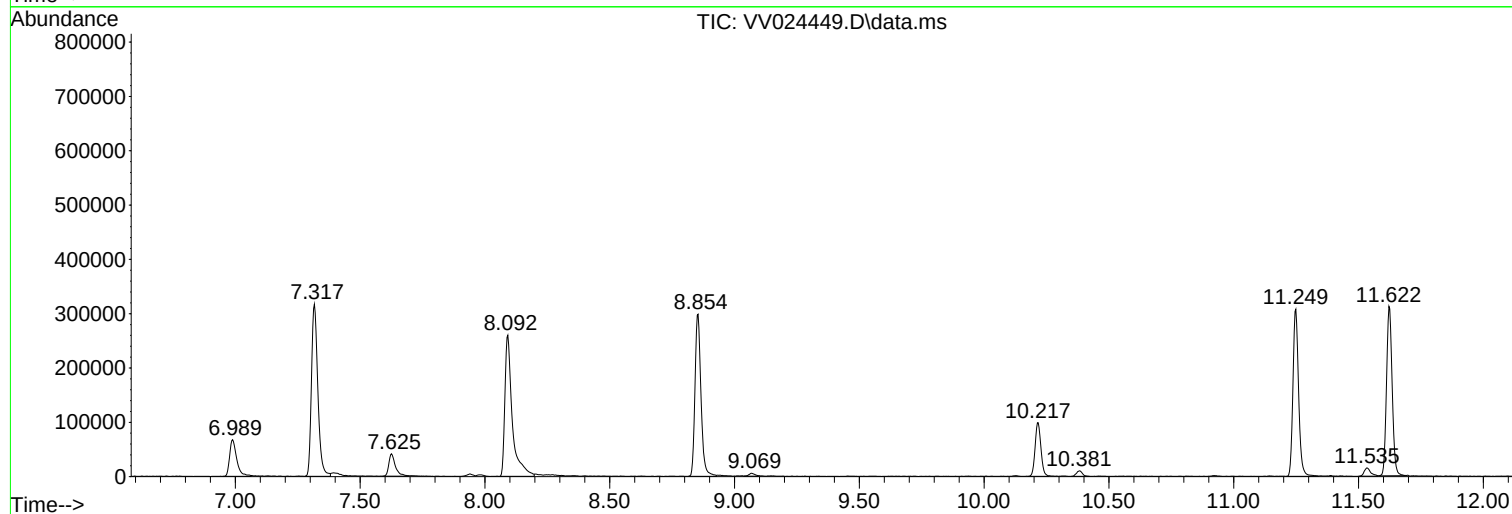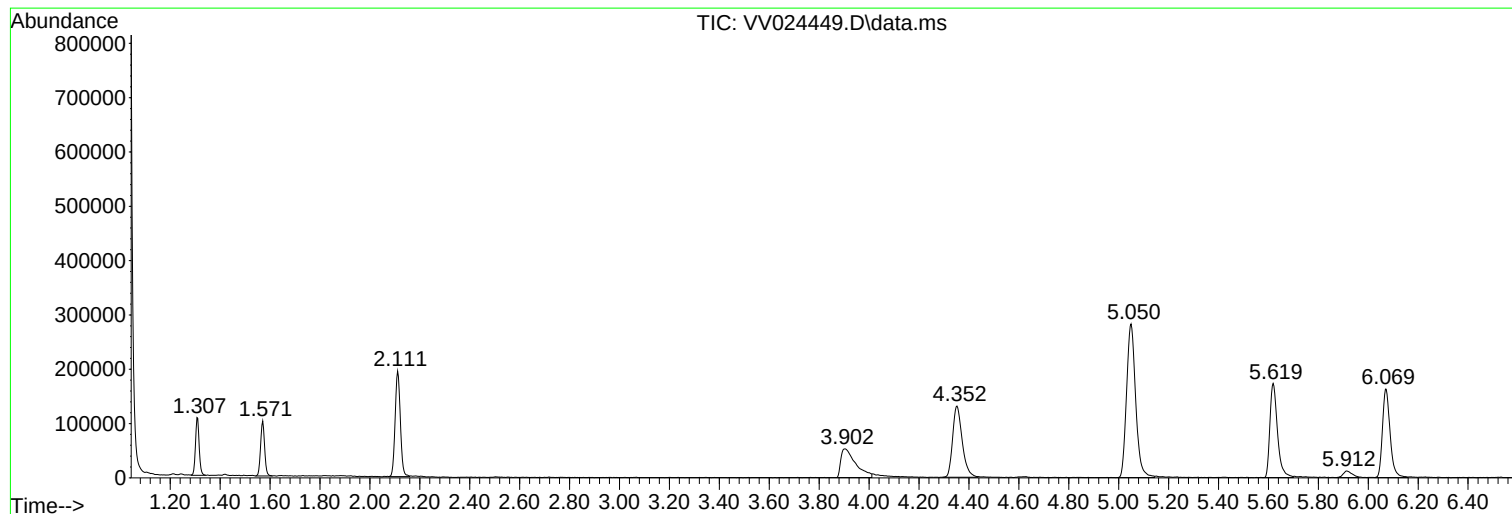

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024449.D
Acq On : 26 Jan 2022 19:06
Operator : SY/MD
Sample : N1275-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024449.D
Acq On : 26 Jan 2022 19:06
Operator : SY/MD
Sample : N1275-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc