
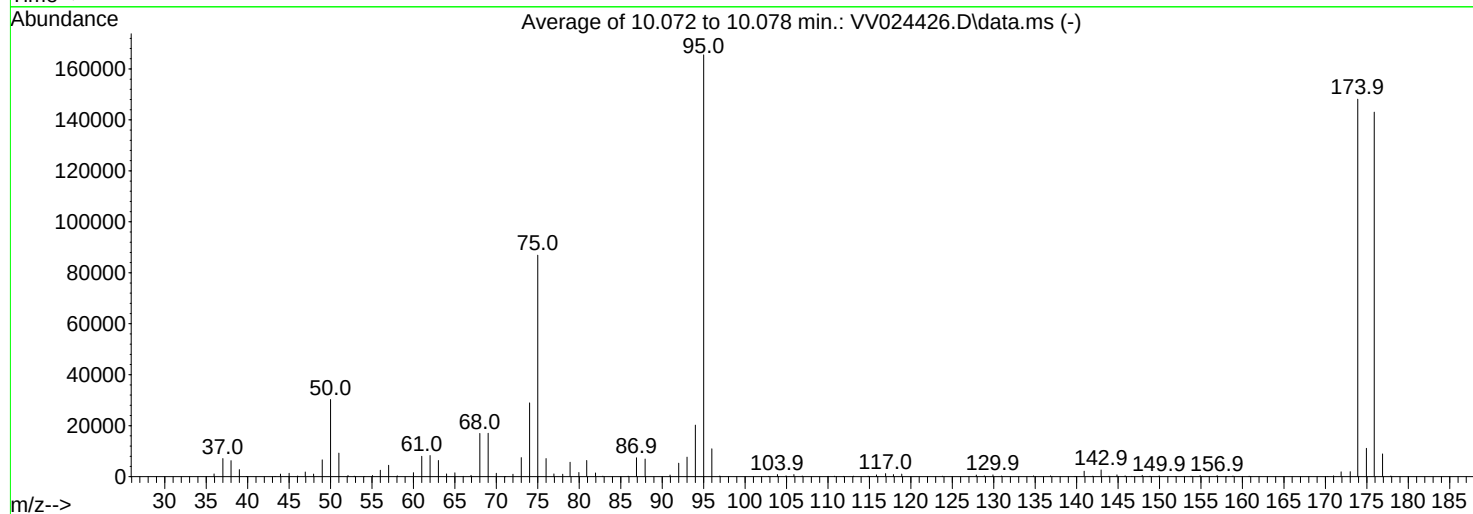


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
 Data File : VV024426.D
 Acq On : 26 Jan 2022 08:50
 Operator : SY/MD
 Sample : BFB263
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB263

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jan 28 03:20:33 2022

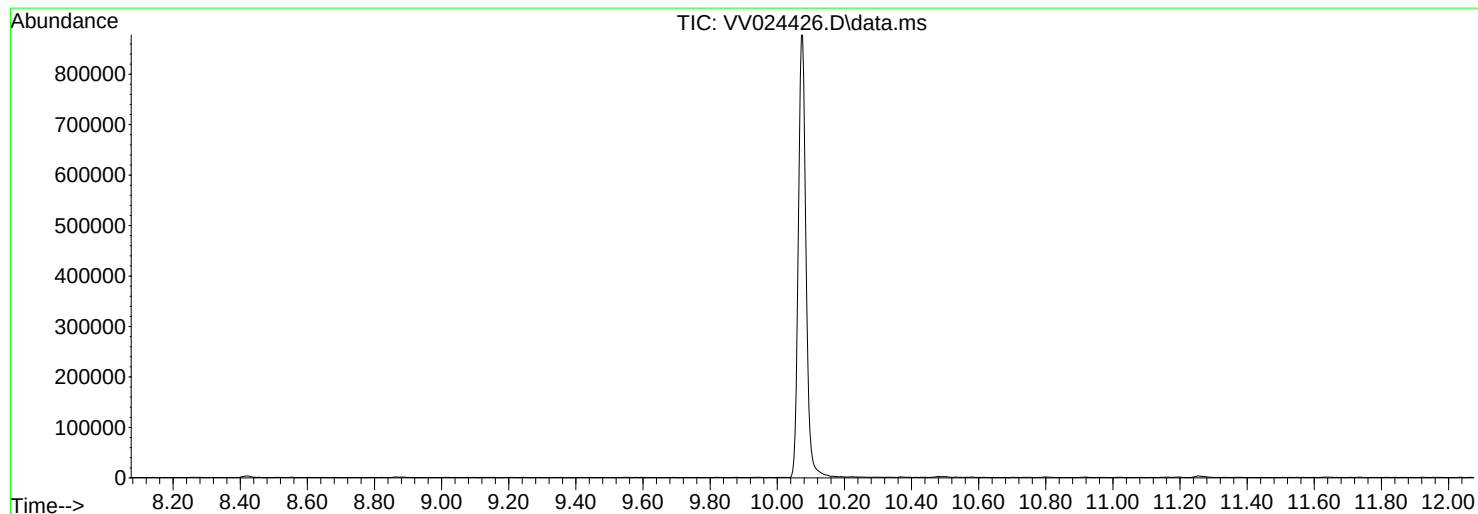

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	30269	PASS
75	95	30	80	52.5	86901	PASS
95	95	100	100	100.0	165525	PASS
96	95	5	9	6.6	10935	PASS
173	174	0.00	2	1.3	1977	PASS
174	95	50	120	89.5	148096	PASS
175	174	5	9	7.5	11149	PASS
176	174	95	105	96.6	143061	PASS
177	176	5	10	6.2	8941	PASS

m/z	Abundance
36.00	1041.0
37.00	6569.0
38.00	5781.0
39.00	2499.0
40.00	260.0
44.00	1249.0
45.00	1235.0
46.00	308.0
47.00	1735.0
48.00	1007.0
49.00	5740.0
50.00	27792.0
51.00	8281.0
52.10	432.0
52.80	161.0
54.10	123.0
55.00	395.0
56.00	2296.0
57.00	4051.0
58.00	295.0
60.00	1474.0
61.00	7270.0
62.00	7844.0
63.00	6074.0
64.00	833.0
65.00	1358.0
66.00	155.0
67.00	485.0
68.00	15503.0
69.00	15372.0
70.00	1236.0
72.00	837.0
73.00	7058.0
74.00	26384.0
75.00	79744.0
76.00	6533.0
76.90	1101.0
78.00	865.0
78.90	4998.0
80.00	1469.0
80.90	6002.0
81.90	1369.0
82.90	161.0
85.90	209.0
86.90	6896.0
88.00	6072.0
90.90	583.0
92.00	4797.0
93.00	7072.0
94.00	18704.0
95.00	154496.0
96.00	9964.0
97.00	255.0
102.80	157.0
103.90	761.0
105.00	232.0
105.90	767.0
106.90	273.0
110.10	132.0
110.80	168.0
111.80	149.0
113.10	153.0
114.80	212.0
115.90	622.0
116.90	1115.0
117.90	790.0
118.90	990.0
123.80	153.0
127.90	658.0
128.90	306.0
129.90	713.0
130.80	263.0
134.70	295.0
136.80	292.0
139.80	120.0
140.90	1977.0
142.00	174.0
143.00	2321.0
143.80	199.0
144.90	601.0
145.90	260.0
146.60	105.0
147.90	499.0
148.80	169.0
149.90	230.0
153.00	137.0
153.80	152.0
154.90	431.0
156.90	400.0
158.00	117.0
158.80	214.0
161.00	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

171.00	340.0
171.90	1790.0
173.00	1772.0
173.90	140800.0
174.90	10260.0
175.90	137216.0
176.90	8819.0
177.90	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	1185.0
37.00	7300.0
38.00	6570.0
39.00	2861.0
40.00	263.0
43.30	128.0
44.00	1451.0
45.00	1503.0
46.00	269.0
46.90	1892.0
47.90	1049.0
49.00	6739.0
50.00	31312.0
51.00	9542.0
52.10	479.0
52.90	221.0
55.00	453.0
56.00	2631.0
57.00	4565.0
58.10	338.0
60.00	1653.0
61.00	8228.0
62.00	8600.0
63.00	6460.0
64.00	1064.0
65.00	1552.0
66.00	161.0
66.90	538.0
68.00	17456.0
69.00	17464.0
70.00	1384.0
72.00	984.0
73.00	7712.0
74.00	29800.0
75.00	89816.0
76.00	7371.0
76.90	1124.0
78.00	968.0
78.90	5849.0
80.00	1651.0
80.90	6570.0
81.90	1480.0
82.80	187.0
85.90	183.0
86.90	7694.0
88.00	7180.0
91.00	616.0
92.00	5530.0
93.00	7895.0
94.00	20944.0
95.00	171072.0
96.00	11267.0
96.90	264.0
102.80	136.0
103.90	854.0
105.00	299.0
105.90	866.0
106.90	272.0
110.00	143.0
110.80	205.0
111.80	148.0
113.10	179.0
114.90	197.0
115.80	729.0
117.00	1272.0
117.90	843.0
118.90	1022.0
123.80	181.0
127.90	646.0
128.90	355.0
129.90	771.0
131.00	273.0
134.90	314.0
136.80	318.0
139.80	168.0
140.90	2268.0
141.90	187.0
142.90	2743.0
143.90	214.0
144.80	714.0
145.80	315.0
146.60	117.0
147.90	501.0
148.90	191.0
149.90	328.0
151.90	107.0
153.10	140.0
153.80	194.0
154.90	434.0
157.00	456.0
158.80	281.0
160.80	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

171.00	358.0
171.90	1966.0
173.00	2047.0
173.90	153024.0
175.00	11557.0
175.90	147584.0
176.90	9193.0
177.90	281.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	1247.0
37.00	7460.0
38.00	6586.0
39.00	2969.0
39.90	305.0
43.30	116.0
44.00	1445.0
45.00	1602.0
46.20	254.0
46.90	1830.0
47.90	1053.0
49.00	7230.0
50.00	31704.0
51.00	9878.0
52.10	435.0
52.90	253.0
55.10	424.0
56.00	2699.0
57.00	4679.0
58.10	305.0
60.00	1695.0
61.00	8496.0
62.00	8487.0
63.00	6461.0
64.00	1228.0
65.00	1549.0
66.00	139.0
66.90	505.0
68.00	17904.0
69.00	18200.0
70.00	1392.0
71.00	104.0
72.00	986.0
73.00	7731.0
74.00	30648.0
75.00	91144.0
76.00	7483.0
77.00	1022.0
78.00	972.0
78.90	6069.0
79.90	1762.0
80.90	6450.0
82.00	1406.0
82.80	179.0
85.90	166.0
86.90	7752.0
87.90	7388.0
91.00	647.0
92.00	5418.0
93.00	8001.0
94.00	21056.0
95.00	171008.0
96.00	11575.0
97.00	265.0
102.90	104.0
103.90	844.0
104.90	339.0
105.90	791.0
106.90	229.0
109.90	139.0
110.80	232.0
111.90	146.0
113.10	180.0
114.90	161.0
115.80	753.0
117.00	1243.0
117.90	824.0
118.90	1018.0
123.80	183.0
127.90	622.0
128.80	382.0
129.90	695.0
131.00	259.0
134.80	362.0
136.90	297.0
139.80	180.0
140.90	2191.0
141.90	195.0
142.90	2850.0
144.00	202.0
144.80	749.0
145.80	362.0
146.80	124.0
147.00	128.0
147.90	443.0
148.90	192.0
150.00	355.0
151.90	112.0
153.10	136.0
153.80	209.0
154.90	416.0
157.00	439.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

158.90	294.0
160.80	265.0
170.30	129.0
171.00	351.0
171.90	1982.0
173.00	2112.0
173.90	150464.0
175.00	11631.0
175.90	144384.0
176.90	8812.0
177.90	301.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
35.80	116.0
39.80	195.0
43.90	402.0
45.20	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263