

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012623\
 Data File : VW029961.D
 Acq On : 26 Jan 2023 14:10
 Operator : SY/MD
 Sample : VIBLK272
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Quant Time: Jan 27 01:30:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 27 01:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	251610	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	239279	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	123607	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	99803	5.230	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.600%
7) Chloroethane-d5	1.564	69	90006	5.689	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.800%
11) 1,1-Dichloroethene-d2	2.105	63	132249	3.801	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.000%
20) 2-Butanone-d5	3.883	46	171450	50.686	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.380%
24) Chloroform-d	4.336	84	161232	4.606	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%
26) 1,2-Dichloroethane-d4	5.021	65	69900	4.715	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	5.040	84	343838	4.844	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	6.059	67	107475	5.174	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.304	98	294849	4.487	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
43) trans-1,3-Dichloroprop...	7.609	79	34708	4.575	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.082	63	140905	45.621	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.240%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	72747	4.779	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	11.612	152	105353	4.688	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.800%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	15341	6.354	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012623\
Data File : VV029961.D
Acq On : 26 Jan 2023 14:10
Operator : SY/MD
Sample : VIBLK272
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK272

Quant Time: Jan 27 01:30:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 27 01:28:41 2023
Response via : Initial Calibration

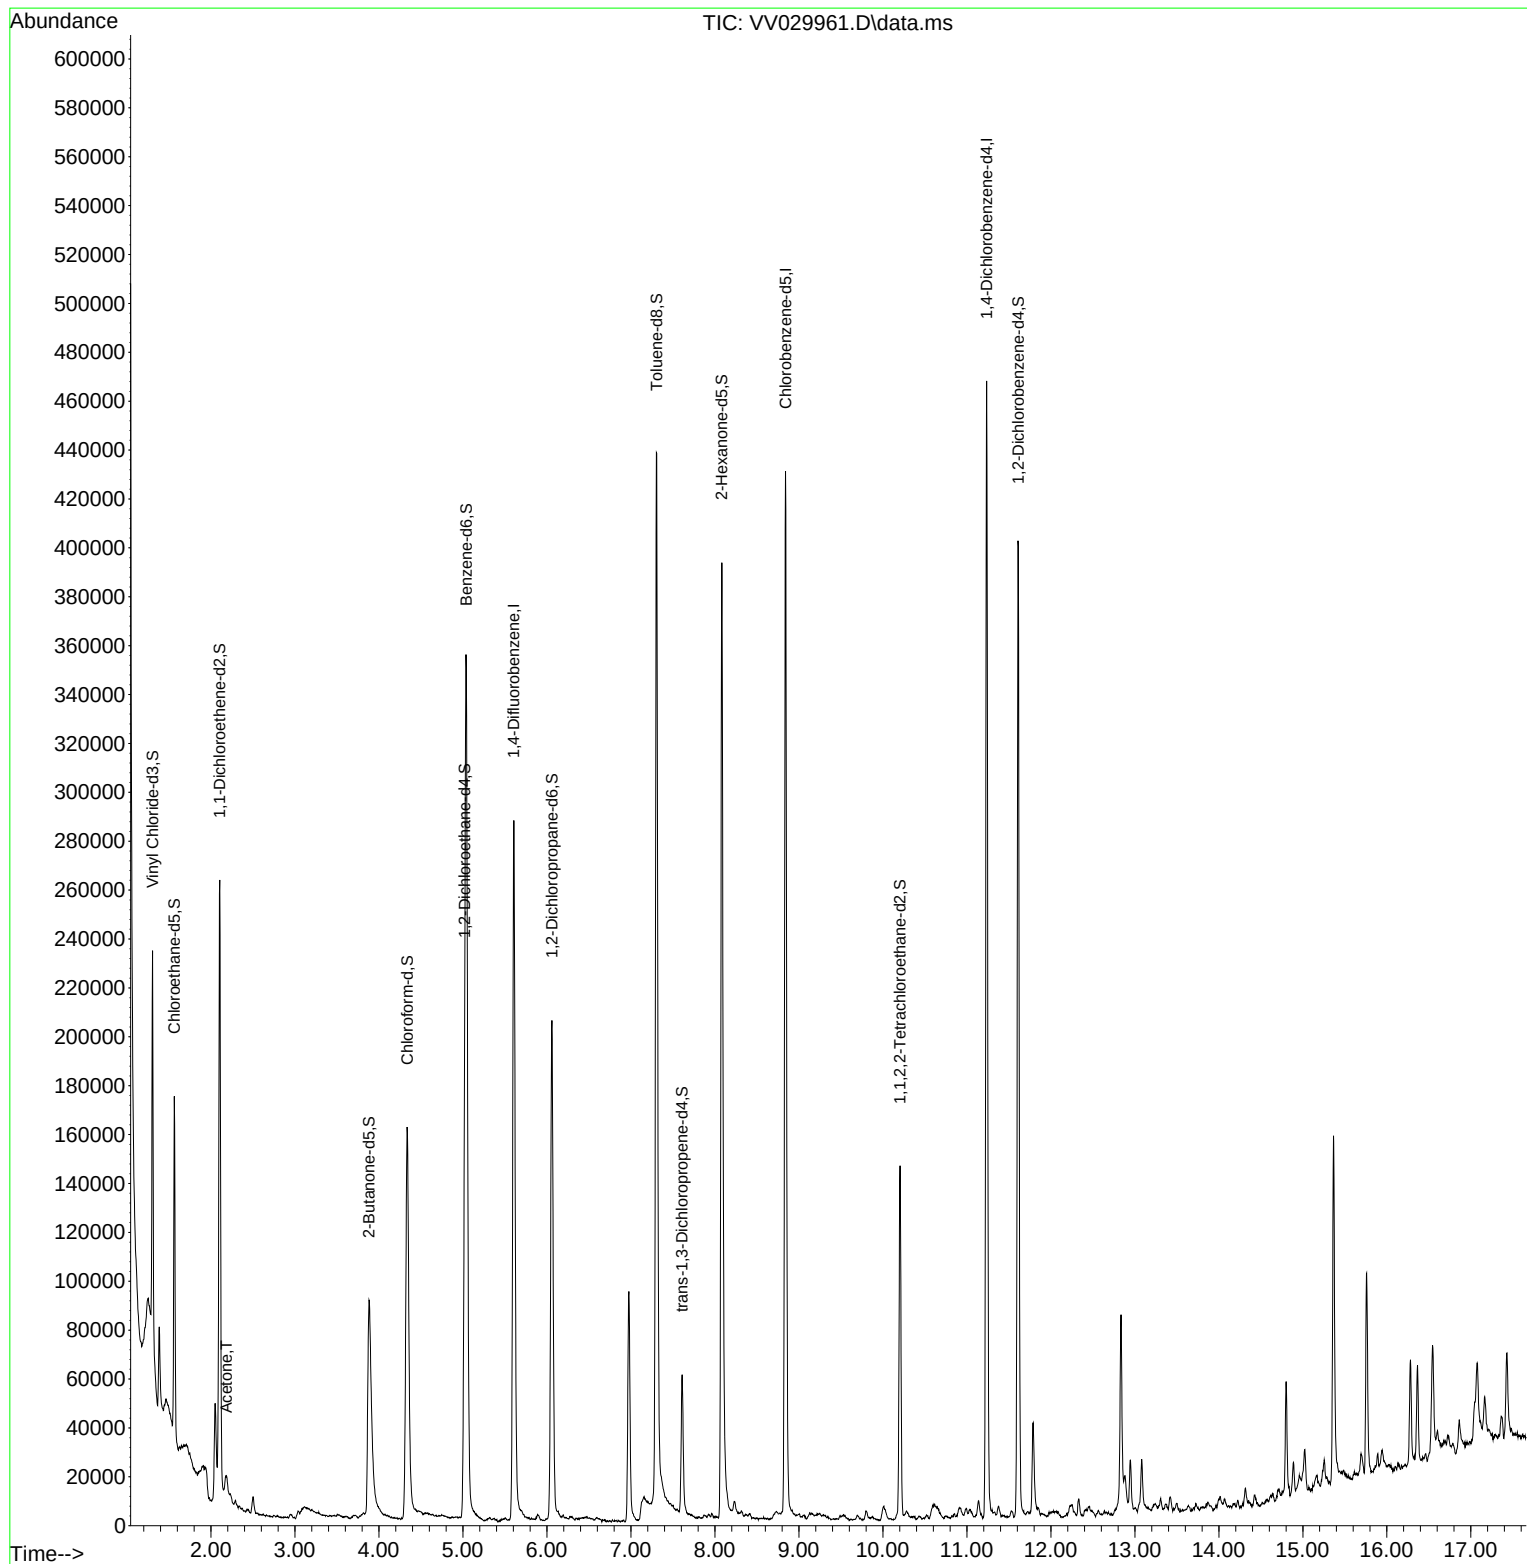

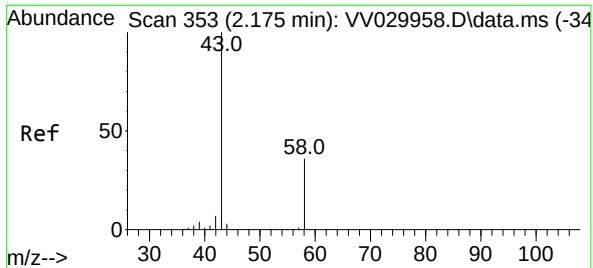

#13
 Acetone
 Concen: 6.354 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. 0.007 min
 Lab File: VV029961.D
 Acq: 26 Jan 2023 14:10

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Tgt Ion: 43 Resp: 15341
 Ion Ratio Lower Upper
 43 100
 58 34.3 0.0 68.8

