

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012623\
 Data File : VW029963.D
 Acq On : 26 Jan 2023 15:15
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Quant Time: Jan 27 01:30:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 27 01:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	241360	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.838	117	231353	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.233	152	118114	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	93767	5.122	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 102.400%		
7) Chloroethane-d5	1.565	69	83666	5.513	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 110.200%		
11) 1,1-Dichloroethene-d2	2.101	63	126097	3.778	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 75.600%		
20) 2-Butanone-d5	3.886	46	173850	53.579	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 107.160%		
24) Chloroform-d	4.330	84	148452	4.421	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 88.400%		
26) 1,2-Dichloroethane-d4	5.018	65	64631	4.544	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 90.800%		
32) Benzene-d6	5.034	84	317880	4.632	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 92.600%		
36) 1,2-Dichloropropane-d6	6.056	67	99760	4.967	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 99.400%		
41) Toluene-d8	7.304	98	264952	4.170	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 83.400%		
43) trans-1,3-Dichloroprop...	7.609	79	31208	4.254	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 85.000%		
46) 2-Hexanone-d5	8.082	63	141132	47.260	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 94.520%		
56) 1,1,2,2-Tetrachloroeth...	10.201	84	69741	4.738	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 94.800%		
66) 1,2-Dichlorobenzene-d4	11.609	152	97465	4.539	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 90.800%		
Target Compounds						
13) Acetone	2.192	43	10609	4.581	ug/L	59
16) Methylene chloride	2.497	84	9047	0.353	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012623\
Data File : VV029963.D
Acq On : 26 Jan 2023 15:15
Operator : SY/MD
Sample : VIBLK273
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Time: Jan 27 01:30:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 27 01:28:41 2023
Response via : Initial Calibration




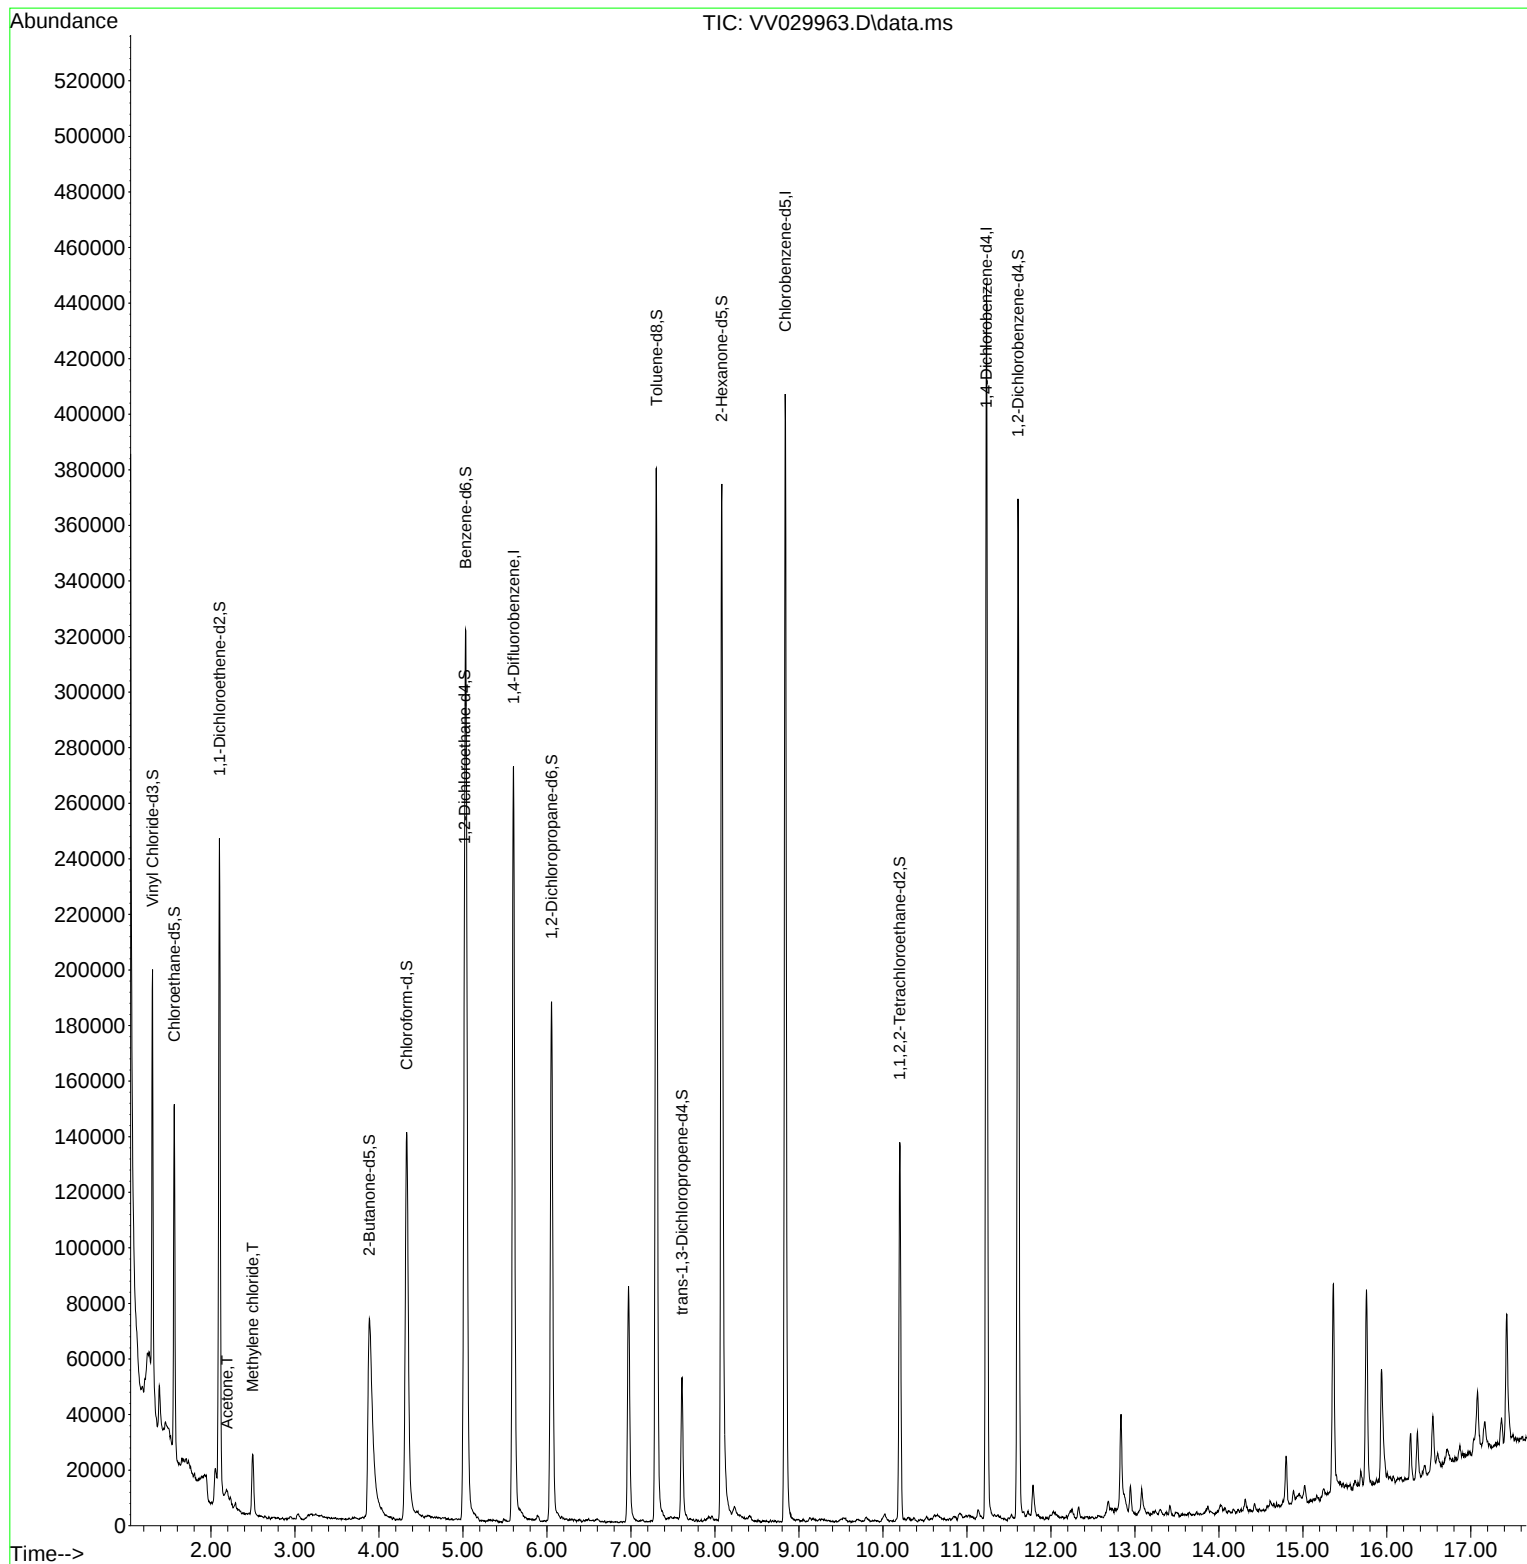


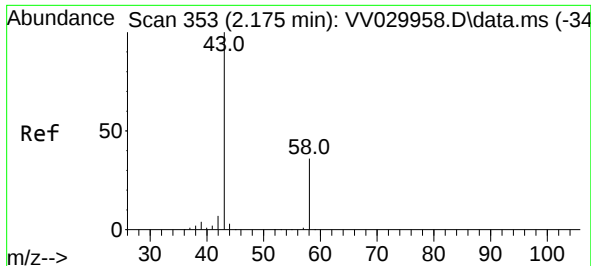

#13
Acetone
Concen: 4.581 ug/L
RT: 2.192 min Scan# 31
Delta R.T. 0.016 min
Lab File: VV029963.D
Acq: 26 Jan 2023 15:15

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Tgt Ion: 43 Resp: 10609
Ion Ratio Lower Upper
43 100
58 10.5 0.0 68.8

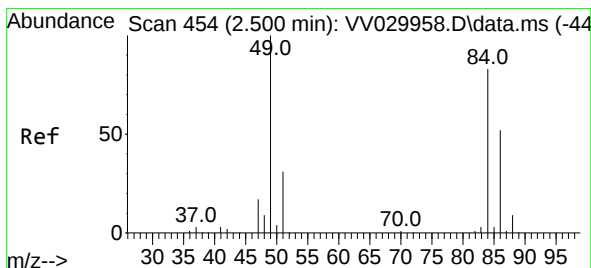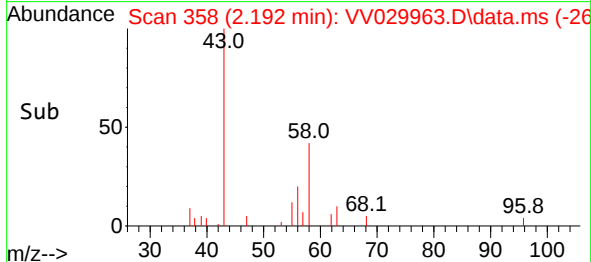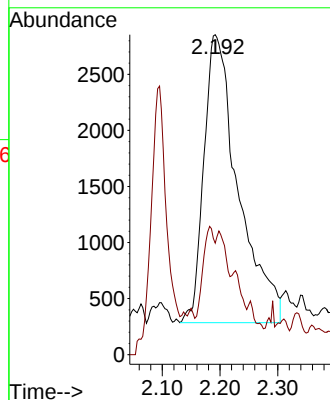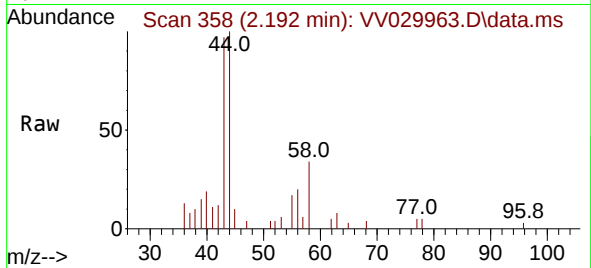

#16
Methylene chloride
Concen: 0.353 ug/L
RT: 2.497 min Scan# 453
Delta R.T. -0.003 min
Lab File: VV029963.D
Acq: 26 Jan 2023 15:15

Tgt Ion: 84 Resp: 9047
Ion Ratio Lower Upper
84 100
86 66.1 45.0 83.6
49 126.5 71.5 132.7

