

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012623\
 Data File : VW029964.D
 Acq On : 26 Jan 2023 16:53
 Operator : SY/MD
 Sample : 01315-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B53

Quant Time: Jan 27 01:30:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 27 01:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	237233	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	224369	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	111992	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	90004	5.002	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.000%
7) Chloroethane-d5	1.565	69	80758	5.414	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.200%
11) 1,1-Dichloroethene-d2	2.105	63	116532	3.553	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.000%
20) 2-Butanone-d5	3.883	46	157643	49.429	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.860%
24) Chloroform-d	4.336	84	147187	4.459	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
26) 1,2-Dichloroethane-d4	5.024	65	65075	4.655	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.040	84	319168	4.796	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
36) 1,2-Dichloropropane-d6	6.059	67	98551	5.060	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.307	98	269483	4.373	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.609	79	31647	4.449	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.000%
46) 2-Hexanone-d5	8.082	63	134469	46.431	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.860%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	66174	4.636	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.800%
66) 1,2-Dichlorobenzene-d4	11.612	152	93932	4.613	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.200%
Target Compounds					Qvalue	
13) Acetone	2.179	43	16226	7.128	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012623\
Data File : VV029964.D
Acq On : 26 Jan 2023 16:53
Operator : SY/MD
Sample : 01315-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B53

Quant Time: Jan 27 01:30:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 27 01:28:41 2023
Response via : Initial Calibration

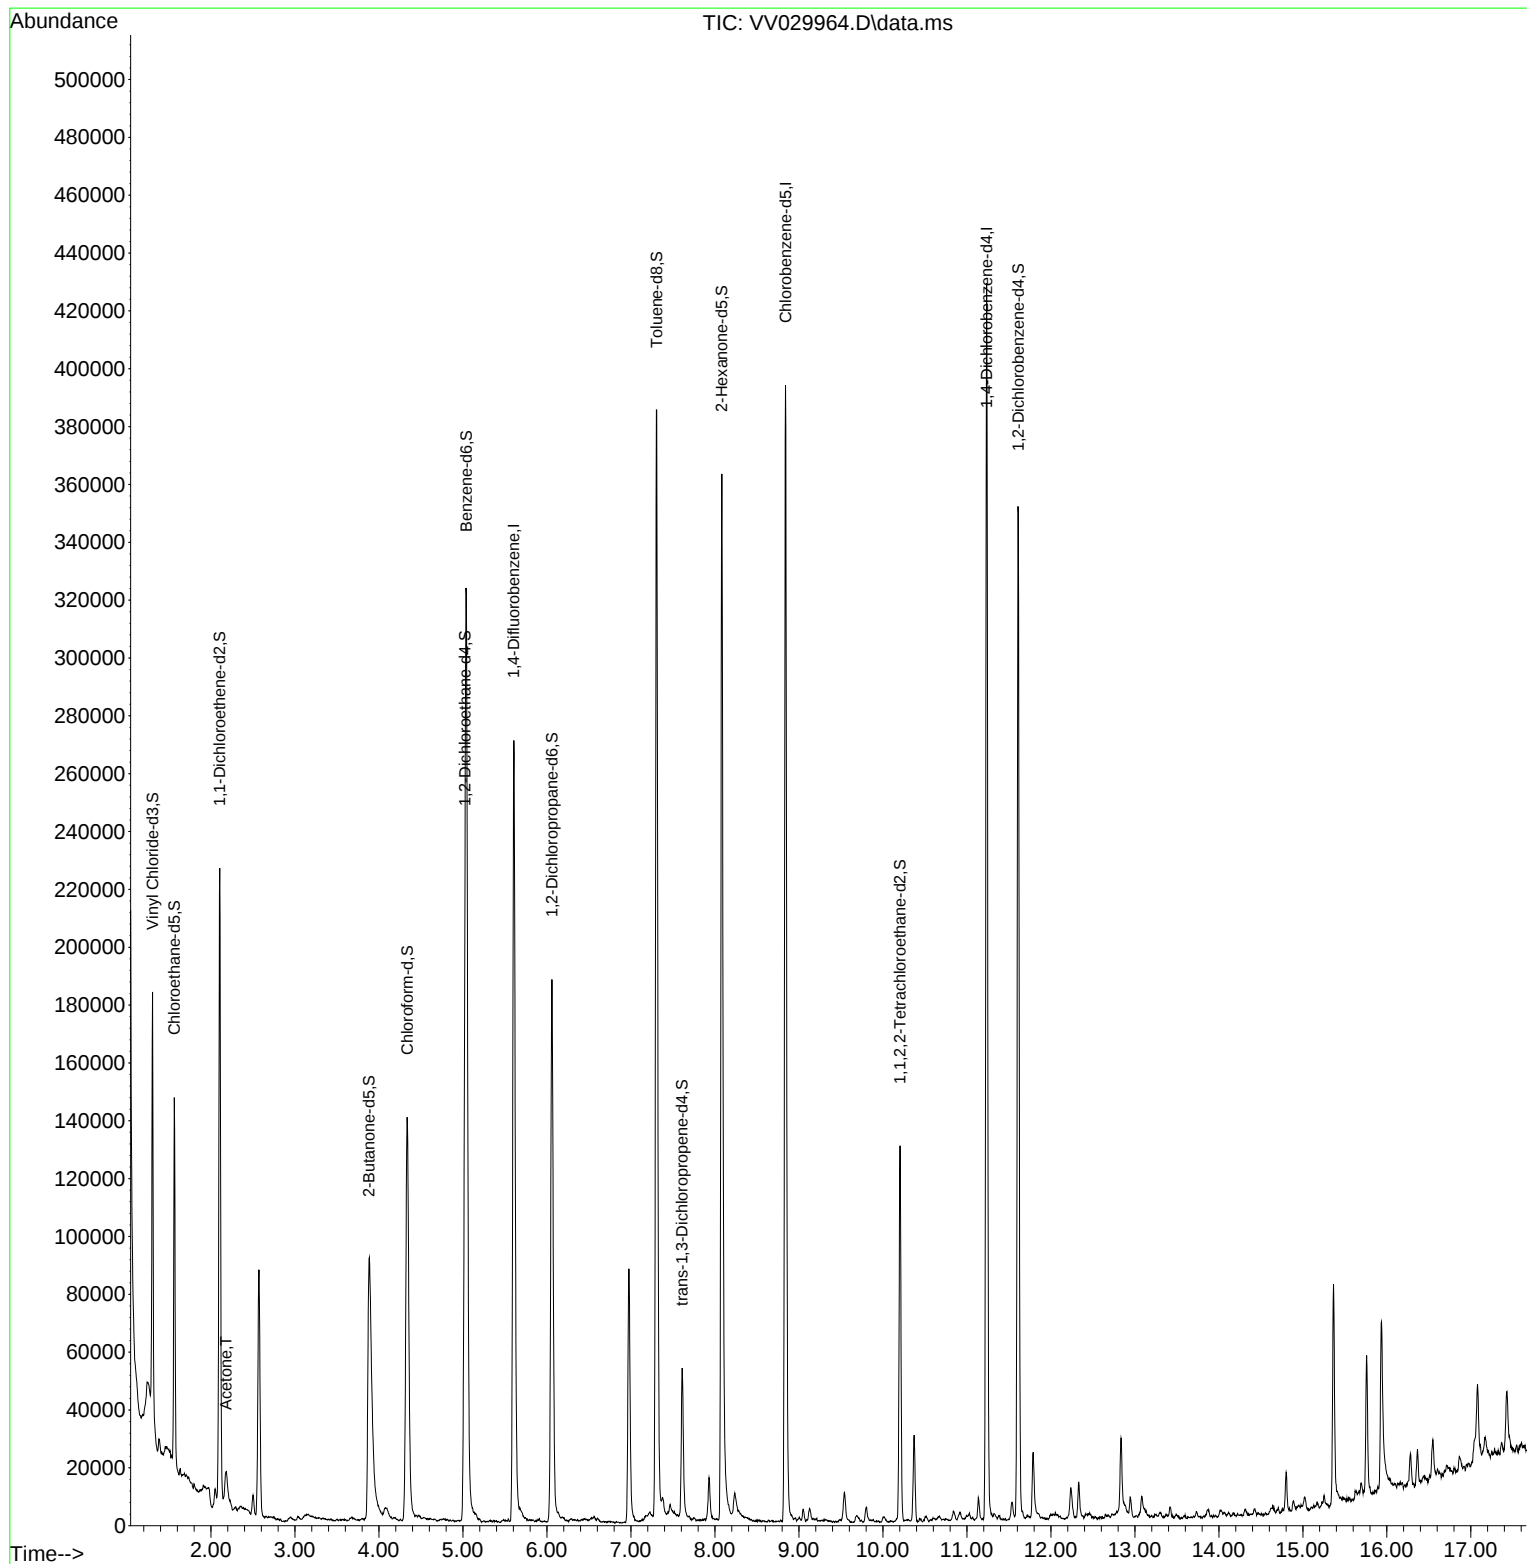

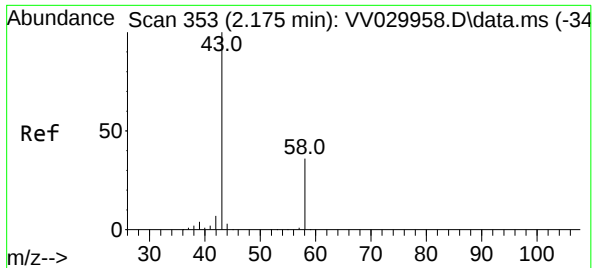

#13
 Acetone
 Concen: 7.128 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV029964.D
 Acq: 26 Jan 2023 16:53

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B53

Tgt Ion: 43 Resp: 16226
 Ion Ratio Lower Upper
 43 100
 58 37.9 0.0 68.8

