


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012623\
Data File : VV029957.D
Acq On : 26 Jan 2023 09:34
Operator : SY/MD
Sample : BFB217
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB217

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Feb 01 00:13:14 2023

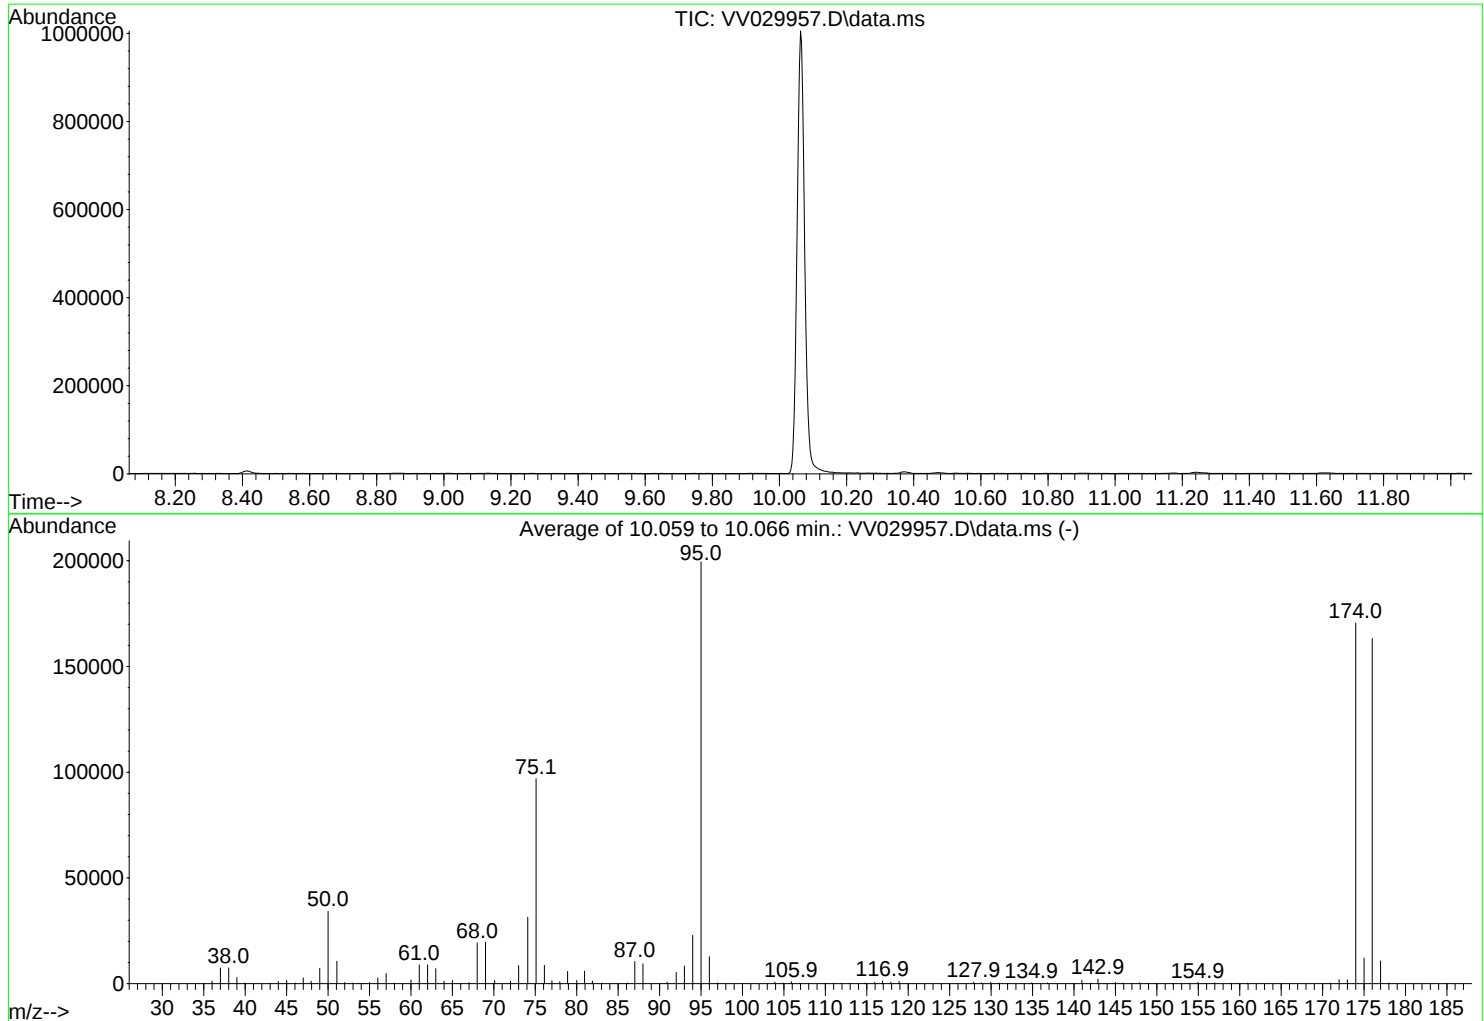

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	34213	PASS
75	95	30	80	48.6	96965	PASS
95	95	100	100	100.0	199509	PASS
96	95	5	9	6.4	12782	PASS
173	174	0.00	2	1.1	1803	PASS
174	95	50	120	85.5	170560	PASS
175	174	5	9	7.1	12036	PASS
176	174	95	105	95.7	163243	PASS
177	176	5	10	6.6	10760	PASS

m/z	Abundance
40.00	285.0
44.00	498.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	1226.0
37.00	7314.0
38.00	7178.0
39.00	2816.0
39.90	549.0
42.90	200.0
44.00	1447.0
45.00	1509.0
46.10	302.0
47.00	2605.0
47.90	1007.0
49.00	6853.0
50.00	32968.0
51.10	10373.0
52.00	560.0
52.90	248.0
55.00	603.0
56.00	2676.0
57.00	4538.0
58.00	239.0
60.00	1753.0
61.00	8614.0
62.00	8597.0
63.00	6857.0
64.00	1217.0
65.00	1366.0
66.10	144.0
67.00	525.0
68.00	18856.0
69.00	19032.0
70.10	1498.0
72.00	1044.0
73.00	8411.0
74.10	30000.0
75.10	94072.0
76.10	8416.0
77.00	1405.0
77.90	887.0
78.90	5399.0
80.00	1400.0
81.00	5616.0
81.90	1176.0
83.10	246.0
86.10	251.0
87.00	9886.0
88.00	9292.0
90.90	612.0
92.00	5209.0
93.00	8013.0
94.00	21928.0
95.00	191872.0
96.00	12437.0
97.00	348.0
103.90	712.0
104.90	276.0
105.90	780.0
106.90	249.0
109.90	102.0
110.90	118.0
111.90	127.0
112.90	128.0
114.80	191.0
115.90	601.0
116.90	1240.0
117.90	616.0
118.90	989.0
127.90	728.0
128.80	340.0
129.90	601.0
131.00	260.0
134.90	369.0
136.80	284.0
141.00	1461.0
142.00	222.0
142.90	1954.0
143.80	159.0
145.00	620.0
145.90	339.0
146.80	120.0
147.90	476.0
148.90	154.0
149.80	181.0
152.90	170.0
153.90	104.0
155.00	507.0
157.00	293.0
158.80	133.0
160.90	226.0
170.90	222.0
172.00	1741.0
173.00	1664.0
174.00	159744.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

175.00	11538.0
176.00	152832.0
177.00	10120.0
178.00	299.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	1266.0
37.00	7671.0
38.00	7714.0
39.00	2977.0
39.90	622.0
42.90	173.0
44.00	1531.0
45.00	1530.0
46.10	295.0
47.00	2867.0
48.00	1242.0
49.00	7458.0
50.00	35440.0
51.00	10945.0
52.00	566.0
52.90	255.0
53.70	118.0
55.00	636.0
56.00	2814.0
57.00	4947.0
57.90	228.0
60.00	1777.0
61.00	9261.0
62.00	9194.0
63.00	7431.0
64.00	1158.0
65.00	1556.0
66.10	155.0
67.00	568.0
68.00	19984.0
69.00	20224.0
70.10	1618.0
72.00	1119.0
73.00	8749.0
74.10	32440.0
75.10	100512.0
76.10	8989.0
77.00	1541.0
78.00	965.0
78.90	5956.0
80.00	1592.0
81.00	6064.0
81.90	1271.0
83.10	198.0
86.10	304.0
87.00	10776.0
88.00	9811.0
90.90	707.0
92.00	5558.0
93.00	8689.0
94.00	23680.0
95.00	206976.0
96.00	13216.0
97.00	377.0
103.90	797.0
104.90	302.0
105.90	916.0
106.90	245.0
108.00	117.0
110.00	114.0
111.00	147.0
111.90	171.0
112.80	157.0
114.70	211.0
116.00	657.0
116.90	1356.0
117.90	697.0
118.90	1138.0
123.70	113.0
127.90	754.0
128.80	373.0
129.90	673.0
131.00	303.0
134.90	405.0
136.80	363.0
140.10	138.0
140.90	1651.0
142.10	241.0
142.90	2213.0
143.90	170.0
145.00	652.0
145.90	338.0
146.80	161.0
147.90	490.0
148.90	158.0
149.80	172.0
153.00	189.0
153.80	154.0
154.90	575.0
155.80	117.0
157.00	374.0
158.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

161.00	255.0
170.90	231.0
172.00	1962.0
173.00	1887.0
174.00	176704.0
175.00	12447.0
176.00	168832.0
177.00	11162.0
178.00	299.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	1168.0
37.00	7226.0
38.00	7375.0
39.00	2965.0
39.90	603.0
42.90	151.0
44.00	1444.0
45.00	1438.0
46.00	224.0
47.00	2747.0
48.00	1280.0
49.00	7360.0
50.00	34232.0
51.00	10476.0
52.00	462.0
53.00	220.0
53.80	117.0
54.20	103.0
55.00	571.0
56.00	2624.0
57.00	4831.0
57.90	226.0
60.00	1688.0
61.00	8765.0
62.00	8746.0
63.00	7162.0
64.00	997.0
65.00	1659.0
66.10	177.0
67.00	531.0
68.00	18952.0
69.00	19344.0
70.10	1496.0
72.00	1112.0
73.00	8406.0
74.10	31720.0
75.10	96312.0
76.10	8563.0
77.00	1450.0
78.00	991.0
78.90	5886.0
80.00	1577.0
80.90	5966.0
81.90	1190.0
83.10	165.0
86.20	290.0
87.00	10639.0
88.00	9099.0
90.90	718.0
92.00	5253.0
93.00	8371.0
94.00	23056.0
95.00	199680.0
96.00	12692.0
97.00	365.0
103.90	810.0
104.90	297.0
105.90	977.0
107.00	223.0
108.00	138.0
110.00	105.0
111.00	167.0
111.80	195.0
112.80	154.0
114.70	193.0
116.00	629.0
116.90	1224.0
117.90	674.0
118.90	1165.0
123.70	139.0
127.90	710.0
128.90	349.0
130.00	733.0
130.90	340.0
134.90	401.0
136.80	399.0
139.90	152.0
140.90	1718.0
142.10	206.0
142.90	2224.0
143.90	169.0
145.00	558.0
145.90	305.0
146.90	141.0
147.90	437.0
148.90	134.0
149.80	166.0
151.90	108.0
153.00	176.0
153.80	165.0
154.90	502.0
155.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

157.00	380.0
158.80	147.0
160.90	252.0
170.90	221.0
172.00	2044.0
173.00	1859.0
174.00	175232.0
175.00	12122.0
176.00	168064.0
177.00	10997.0
178.00	287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217