

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012624\
 Data File : VW033880.D
 Acq On : 26 Jan 2024 12:21
 Operator : SY/MD
 Sample : P1238-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH703

Quant Time: Jan 29 02:01:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 29 01:58:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	211684	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	195467	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	96892	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	74039	45.509	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.020%		
7) Chloroethane-d5	1.529	69	59399	46.104	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.200%		
11) 1,1-Dichloroethene-d2	2.060	65	33475	47.810	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.620%		
21) 2-Butanone-d5	3.783	46	86630	77.633	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	77.630%		
24) Chloroform-d	4.249	84	126737	43.566	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.140%		
26) 1,2-Dichloroethane-d4	4.941	65	86532	46.037	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.080%		
32) Benzene-d6	4.960	84	248194	44.663	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.320%		
36) 1,2-Dichloropropane-d6	5.989	67	75572	41.315	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.620%		
41) Toluene-d8	7.243	98	225146	44.967	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.940%		
43) trans-1,3-Dichloroprop...	7.555	79	38811	42.931	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.860%		
47) 2-Hexanone-d5	8.024	63	68954	90.880	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.880%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	101700	43.551	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.100%		
66) 1,2-Dichlorobenzene-d4	11.561	152	85475	46.496	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.000%		
Target Compounds					Qvalue	
38) Bromodichloromethane	6.439	83	3112	1.506	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012624\
Data File : VV033880.D
Acq On : 26 Jan 2024 12:21
Operator : SY/MD
Sample : P1238-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH703

Quant Time: Jan 29 02:01:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 29 01:58:36 2024
Response via : Initial Calibration

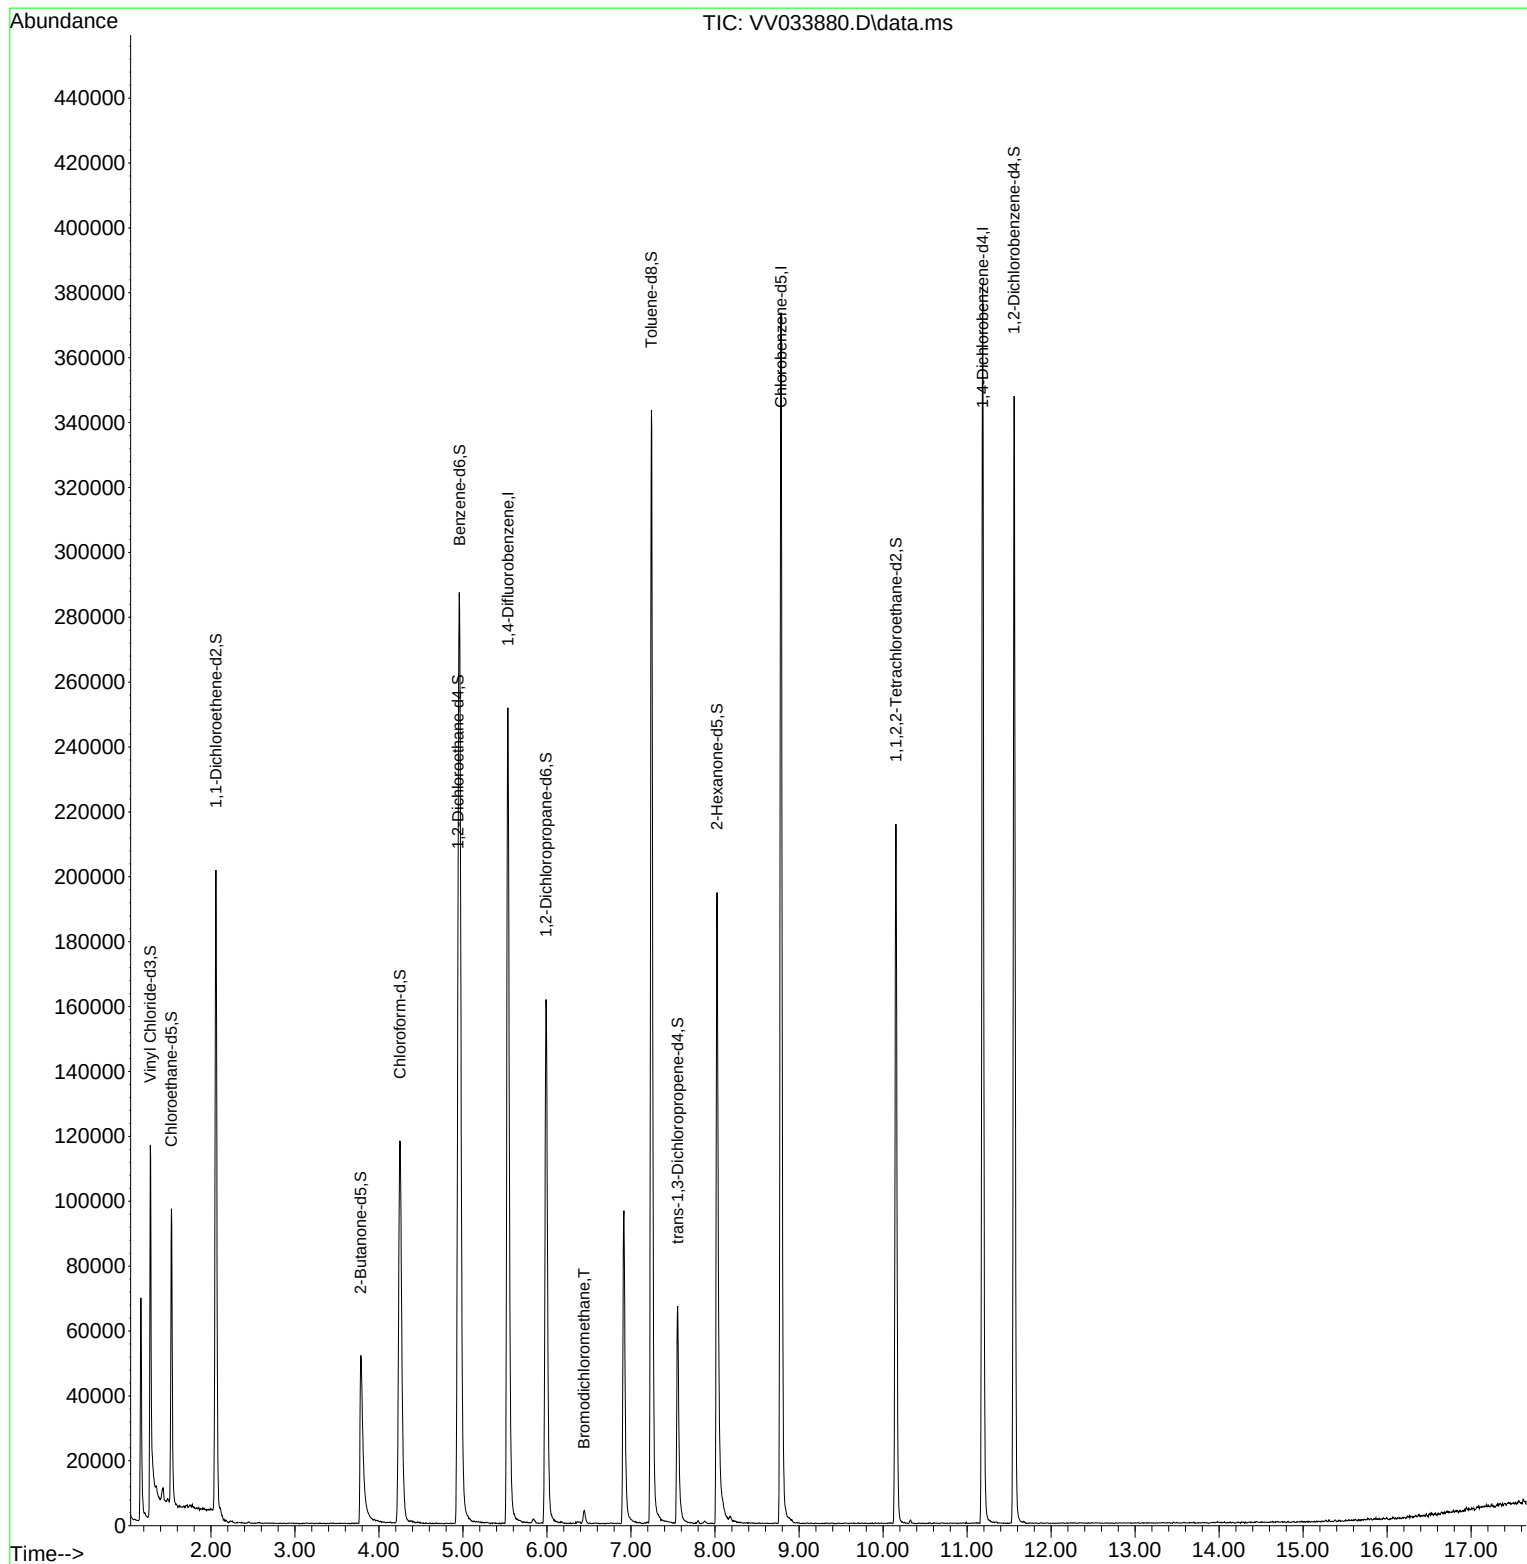

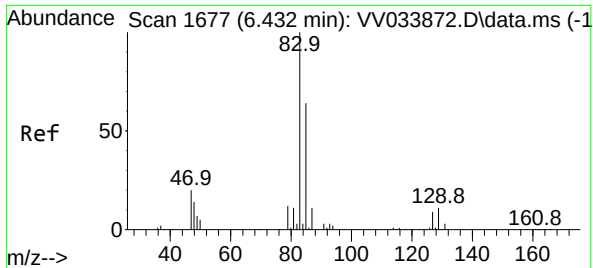

#38
 Bromodichloromethane
 Concen: 1.506 ug/L
 RT: 6.439 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: VV033880.D
 Acq: 26 Jan 2024 12:21

Instrument :
 MSVOA_V
 ClientSampleId :
 BH703

Tgt Ion: 83 Resp: 3112
 Ion Ratio Lower Upper
 83 100
 85 66.2 45.1 83.7
 127 9.5 6.6 9.8

