


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012624\
Data File : VV033871.D
Acq On : 26 Jan 2024 08:35
Operator : SY/MD
Sample : BFB258
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB258

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Mon Jan 29 01:58:36 2024

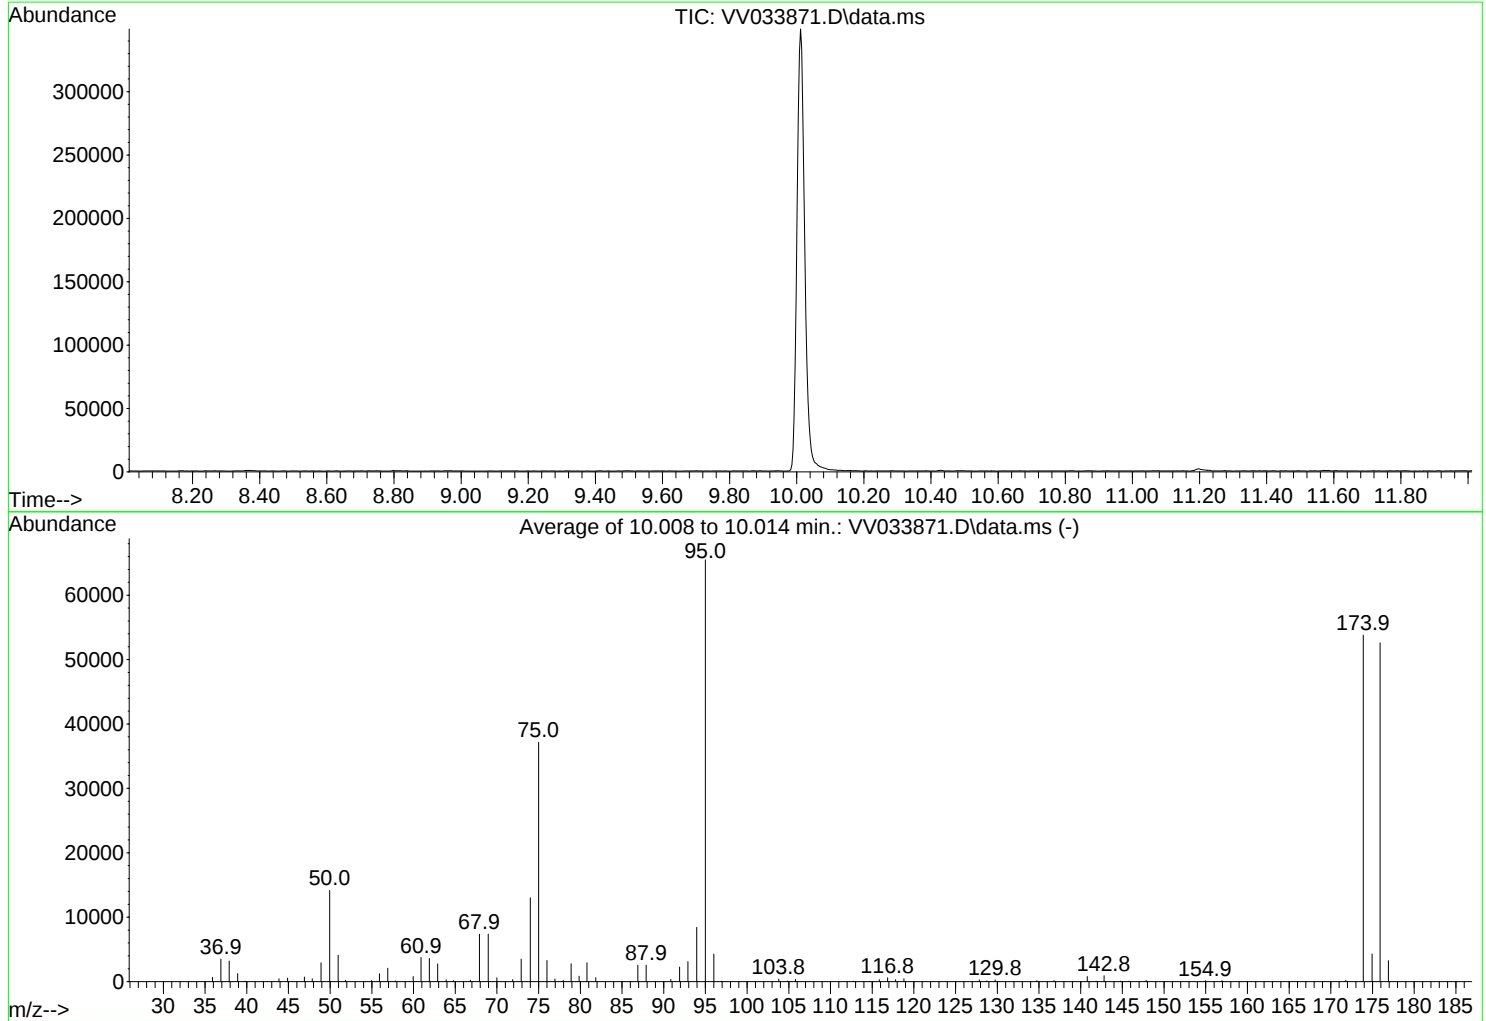

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	14161	PASS
75	95	30	80	56.7	37155	PASS
95	95	100	100	100.0	65488	PASS
96	95	5	9	6.5	4286	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.1	53797	PASS
175	174	5	9	8.0	4305	PASS
176	174	95	105	97.8	52608	PASS
177	176	5	10	6.2	3250	PASS

m/z	Abundance
39.80	537.0
43.80	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
35.90	672.0
36.90	3525.0
37.90	3211.0
38.90	1324.0
39.80	632.0
43.90	592.0
44.90	520.0
46.90	824.0
47.90	461.0
48.90	2921.0
50.00	14337.0
50.90	4093.0
51.90	200.0
55.00	179.0
55.90	1238.0
56.90	2077.0
57.80	117.0
60.00	794.0
60.90	3764.0
61.90	3612.0
62.90	2705.0
63.90	326.0
64.80	134.0
66.80	233.0
67.90	7325.0
69.00	7256.0
70.00	620.0
71.90	358.0
72.90	3449.0
74.00	12938.0
75.00	36608.0
76.00	3251.0
76.90	467.0
77.80	233.0
78.90	2680.0
79.80	845.0
80.80	2933.0
81.90	663.0
86.90	2442.0
87.90	2532.0
90.90	354.0
91.90	2218.0
92.90	2968.0
94.00	8366.0
95.00	64104.0
96.00	4276.0
97.20	102.0
103.80	362.0
104.90	104.0
105.80	355.0
115.80	256.0
116.90	591.0
117.80	330.0
118.80	427.0
127.90	306.0
128.80	136.0
129.80	276.0
134.70	193.0
136.80	182.0
140.80	774.0
142.80	885.0
144.80	102.0
147.80	175.0
155.00	151.0
157.00	136.0
171.80	204.0
173.90	51472.0
174.90	4120.0
175.90	50416.0
176.90	3160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
35.90	717.0
36.90	3597.0
37.90	3320.0
38.90	1275.0
39.80	634.0
43.90	632.0
44.90	567.0
46.90	737.0
47.90	446.0
48.90	3028.0
49.90	14638.0
50.90	4209.0
51.90	203.0
55.00	190.0
55.90	1270.0
56.90	2155.0
57.80	148.0
60.00	854.0
60.90	3886.0
61.90	3724.0
62.90	2881.0
63.90	318.0
64.80	183.0
66.80	240.0
67.90	7549.0
69.00	7519.0
70.00	616.0
71.90	333.0
72.90	3567.0
74.00	13474.0
75.00	38392.0
76.00	3404.0
77.00	427.0
78.00	259.0
78.90	2886.0
79.80	882.0
80.80	3011.0
81.90	627.0
86.10	112.0
86.90	2660.0
87.90	2713.0
90.90	360.0
91.90	2354.0
92.90	3179.0
94.00	8708.0
95.00	67656.0
96.00	4387.0
96.90	117.0
103.80	418.0
104.90	103.0
105.80	361.0
112.70	111.0
114.70	109.0
115.90	330.0
116.90	616.0
117.80	305.0
118.80	458.0
127.90	288.0
128.80	140.0
129.70	300.0
134.70	154.0
136.80	184.0
140.80	820.0
141.80	110.0
142.80	950.0
144.80	107.0
145.80	119.0
147.90	212.0
155.00	156.0
156.90	145.0
171.80	198.0
173.90	55504.0
174.90	4462.0
175.90	54392.0
176.90	3346.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
35.90	629.0
36.90	3380.0
37.90	3099.0
38.90	1119.0
39.80	567.0
43.90	662.0
44.90	555.0
46.90	636.0
47.80	434.0
48.90	2830.0
49.90	13507.0
51.00	4019.0
51.80	169.0
54.80	192.0
55.90	1157.0
56.90	2045.0
57.80	145.0
59.90	758.0
60.90	3624.0
61.90	3490.0
62.90	2674.0
63.90	284.0
64.80	163.0
66.80	205.0
67.90	7178.0
68.90	7347.0
70.00	531.0
71.90	327.0
72.90	3482.0
74.00	12658.0
75.00	36464.0
76.00	3188.0
77.00	389.0
77.90	270.0
78.90	2815.0
79.90	812.0
80.80	2838.0
81.80	598.0
86.90	2572.0
87.90	2469.0
90.80	316.0
91.90	2208.0
92.90	3147.0
93.90	8172.0
95.00	64704.0
96.00	4195.0
96.90	116.0
103.80	409.0
104.80	104.0
105.80	330.0
112.80	103.0
115.80	362.0
116.80	560.0
117.80	290.0
118.80	458.0
127.80	241.0
128.70	139.0
129.70	265.0
134.80	116.0
136.80	144.0
140.80	784.0
141.90	112.0
142.80	904.0
145.80	121.0
147.80	225.0
154.90	143.0
156.90	157.0
171.80	173.0
173.90	54416.0
175.00	4332.0
175.90	53016.0
176.90	3244.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258