

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012721\
 Data File : VV020178.D
 Acq On : 26 Jan 2021 18:54
 Operator : SY/MD
 Sample : VV0127WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012721WMA.M

Title : VOC Analysis

Signal : TIC: VV020178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	506275	529348	15.07%	1.905%
2	1.569	142	149	162	rVB	429615	470821	13.40%	1.695%
3	2.110	307	317	345	rVB	765219	1152680	32.81%	4.149%
4	2.502	435	439	440	rBV4	2432	1730	0.05%	0.006%
5	2.753	512	517	518	rBV5	1543	1110	0.03%	0.004%
6	2.929	570	572	577	rBV3	790	570	0.02%	0.002%
7	2.978	584	587	589	rVB3	856	601	0.02%	0.002%
8	3.036	602	605	607	rBV4	1122	775	0.02%	0.003%
9	3.074	614	617	620	rBV3	983	583	0.02%	0.002%
10	3.328	693	696	699	rVB3	1231	707	0.02%	0.003%
11	3.344	699	701	705	rVB4	952	607	0.02%	0.002%
12	3.460	735	737	740	rVB3	837	510	0.01%	0.002%
13	3.547	762	764	766	rBV3	948	492	0.01%	0.002%
14	3.566	766	770	772	rVV2	1114	727	0.02%	0.003%
15	3.589	775	777	779	rVV3	973	495	0.01%	0.002%
16	3.653	795	797	804	rVB5	1052	973	0.03%	0.004%
17	3.717	815	817	820	rBV2	1127	585	0.02%	0.002%
18	3.894	858	872	915	rBV	254800	779032	22.18%	2.804%
19	4.216	970	972	975	rVB3	1120	535	0.02%	0.002%
20	4.354	997	1015	1039	rBV	571097	1391554	39.61%	5.008%
21	4.537	1070	1072	1078	rVB5	1291	1054	0.03%	0.004%
22	4.566	1078	1081	1082	rBV3	978	535	0.02%	0.002%
23	4.598	1088	1091	1094	rVB3	1366	739	0.02%	0.003%
24	4.891	1179	1182	1185	rBV4	1110	878	0.02%	0.003%
25	4.968	1204	1206	1211	rBV5	882	523	0.01%	0.002%
26	5.051	1214	1232	1267	rBV2	1372683	3512895	100.00%	12.643%
27	5.415	1342	1345	1348	rBV5	1689	1437	0.04%	0.005%
28	5.473	1360	1363	1366	rBV5	1893	1686	0.05%	0.006%
29	5.563	1388	1391	1392	rBV3	829	493	0.01%	0.002%
30	5.621	1396	1409	1441	rBV	1138382	2266342	64.51%	8.157%
31	5.830	1472	1474	1478	rVB5	2177	1291	0.04%	0.005%
32	5.913	1492	1500	1518	rVB7	12536	27227	0.78%	0.098%
33	6.074	1535	1550	1578	rBV	772474	1582579	45.05%	5.696%
34	6.383	1643	1646	1651	rVB6	820	742	0.02%	0.003%
35	6.466	1666	1672	1676	rBV7	1287	1627	0.05%	0.006%
36	6.540	1689	1695	1700	rBV6	1898	2003	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012721\
 Data File : VV020178.D
 Acq On : 26 Jan 2021 18:54
 Operator : SY/MD
 Sample : VV0127WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012721WMA.M
 Title : VOC Analysis

37	6.572	1703	1705	1709	rBV5	916	727	0.02%	0.003%
38	6.598	1710	1713	1715	rVV3	930	534	0.02%	0.002%
39	6.733	1753	1755	1761	rVB6	2304	1821	0.05%	0.007%
40	6.768	1761	1766	1769	rBV6	1048	821	0.02%	0.003%
41	6.794	1769	1774	1776	rBV4	827	818	0.02%	0.003%
42	6.810	1776	1779	1782	rVB4	1253	701	0.02%	0.003%
43	6.990	1824	1835	1862	rVV	435561	785827	22.37%	2.828%
44	7.318	1923	1937	1966	rBV	1631126	2833090	80.65%	10.197%
45	7.624	2022	2032	2051	rBV	305588	528484	15.04%	1.902%
46	7.781	2080	2081	2085	rVB4	1375	592	0.02%	0.002%
47	7.981	2141	2143	2146	rBV4	1418	743	0.02%	0.003%
48	8.090	2167	2177	2214	rBV	975367	1694396	48.23%	6.098%
49	8.669	2354	2357	2361	rVB6	964	725	0.02%	0.003%
50	8.855	2403	2415	2442	rBV	1724863	2794832	79.56%	10.059%
51	9.305	2552	2555	2558	rVV5	1234	733	0.02%	0.003%
52	9.373	2572	2576	2578	rBV3	1154	974	0.03%	0.004%
53	9.620	2650	2653	2656	rBV4	718	504	0.01%	0.002%
54	9.678	2666	2671	2673	rBV4	731	685	0.02%	0.002%
55	9.778	2700	2702	2709	rVB4	1723	1355	0.04%	0.005%
56	9.813	2709	2713	2714	rBV3	1223	676	0.02%	0.002%
57	9.855	2723	2726	2731	rVB5	792	593	0.02%	0.002%
58	9.894	2731	2738	2742	rBV5	661	820	0.02%	0.003%
59	9.945	2744	2754	2757	rBV5	1763	2275	0.06%	0.008%
60	10.003	2766	2772	2775	rBV4	1211	1049	0.03%	0.004%
61	10.064	2786	2791	2794	rBV5	1293	1407	0.04%	0.005%
62	10.096	2798	2801	2803	rBV3	827	511	0.01%	0.002%
63	10.154	2813	2819	2822	rBV4	838	1088	0.03%	0.004%
64	10.222	2826	2840	2856	rBV	1081756	1677314	47.75%	6.037%
65	10.382	2885	2890	2894	rVB7	1414	1562	0.04%	0.006%
66	10.411	2894	2899	2900	rBV2	868	571	0.02%	0.002%
67	10.575	2947	2950	2954	rVB4	1559	1083	0.03%	0.004%
68	10.649	2970	2973	2976	rBV3	818	557	0.02%	0.002%
69	10.739	2997	3001	3002	rBV3	1112	722	0.02%	0.003%
70	10.791	3015	3017	3021	rVV4	723	654	0.02%	0.002%
71	10.865	3034	3040	3044	rBV6	3523	3876	0.11%	0.014%
72	10.929	3057	3060	3069	rVV7	2696	3137	0.09%	0.011%
73	11.112	3113	3117	3120	rBV5	1127	834	0.02%	0.003%
74	11.254	3149	3161	3184	rBV	1859658	2854391	81.25%	10.273%
75	11.415	3208	3211	3215	rVB4	1428	1012	0.03%	0.004%
76	11.579	3258	3262	3263	rBV3	1015	767	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012721\
 Data File : VV020178.D
 Acq On : 26 Jan 2021 18:54
 Operator : SY/MD
 Sample : VV0127WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012721WMA.M

Title : VOC Analysis

77	11.630	3266	3278	3297	rVV	1813841	2795633	79.58%	10.062%
78	11.862	3347	3350	3351	rBV3	873	503	0.01%	0.002%
79	11.961	3378	3381	3383	rBV4	755	540	0.02%	0.002%
80	11.987	3387	3389	3392	rVV3	956	586	0.02%	0.002%
81	12.218	3458	3461	3466	rVB5	1390	1037	0.03%	0.004%
82	12.251	3466	3471	3475	rBV4	1100	1100	0.03%	0.004%
83	12.318	3489	3492	3499	rVB4	1452	1533	0.04%	0.006%
84	12.472	3538	3540	3544	rVB3	1036	666	0.02%	0.002%
85	12.517	3549	3554	3557	rBV3	762	617	0.02%	0.002%
86	12.662	3589	3599	3607	rBV7	5024	8533	0.24%	0.031%
87	12.845	3653	3656	3660	rBV5	1282	1027	0.03%	0.004%
88	12.984	3695	3699	3700	rBV3	975	620	0.02%	0.002%
89	13.276	3778	3790	3798	rBV7	6946	12323	0.35%	0.044%
90	13.312	3798	3801	3806	rVV5	1240	1143	0.03%	0.004%
91	13.341	3808	3810	3813	rVB4	1374	540	0.02%	0.002%
92	13.395	3824	3827	3828	rBV3	1077	604	0.02%	0.002%
93	13.521	3860	3866	3873	rVB5	3992	6329	0.18%	0.023%
94	13.675	3912	3914	3917	rBV3	819	533	0.02%	0.002%
95	13.759	3933	3940	3948	rVB8	5203	7012	0.20%	0.025%
96	13.906	3982	3986	3987	rBV2	1446	947	0.03%	0.003%
97	14.128	4052	4055	4057	rBV4	1223	686	0.02%	0.002%
98	14.250	4091	4093	4095	rBV3	1136	495	0.01%	0.002%
99	14.408	4138	4142	4146	rBV5	1199	1213	0.03%	0.004%
100	14.492	4166	4168	4175	rVB6	1231	736	0.02%	0.003%




Sum of corrected areas: 27784703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012721\
Data File : VV020178.D
Acq On : 26 Jan 2021 18:54
Operator : SY/MD
Sample : VV0127WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

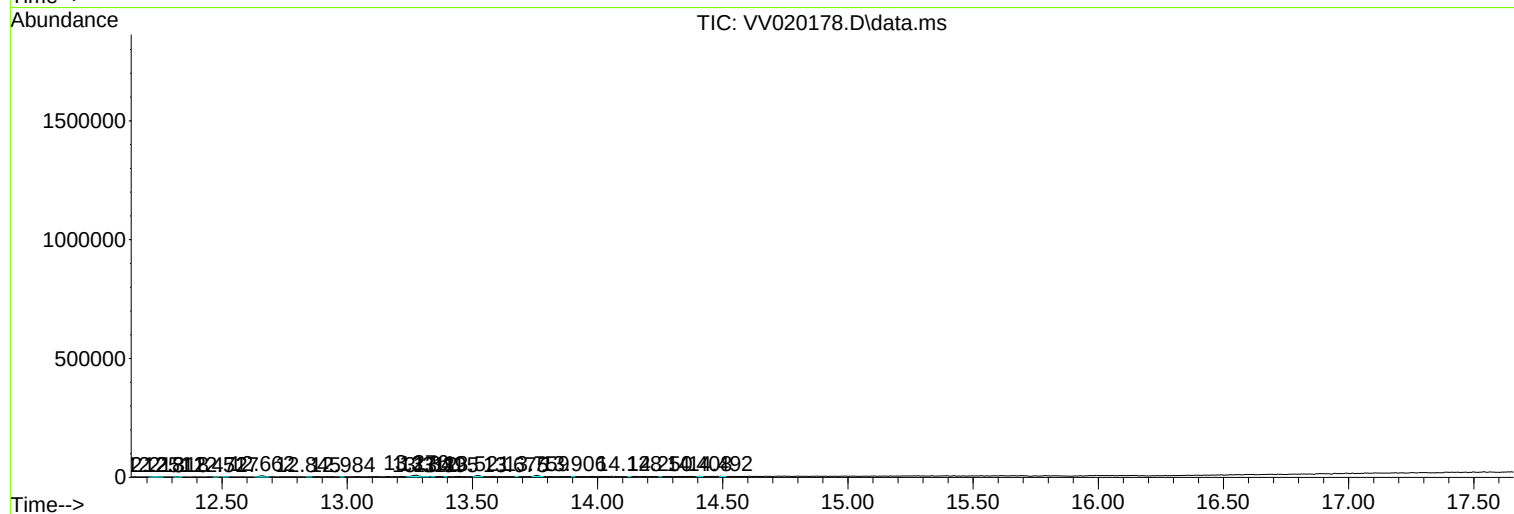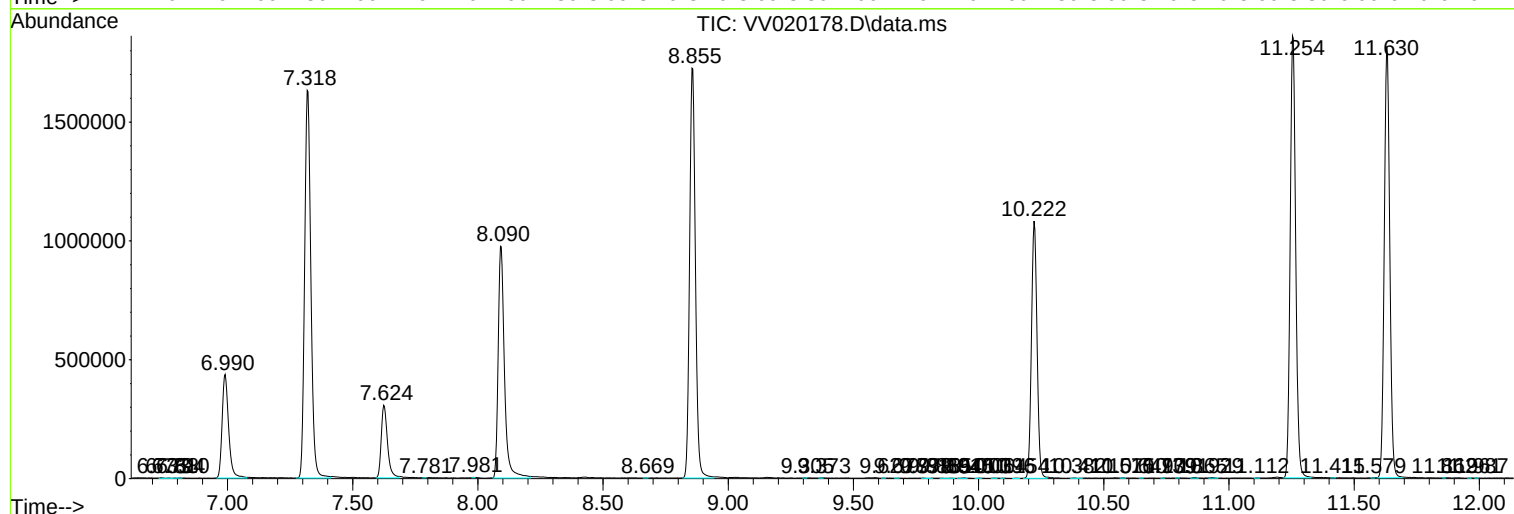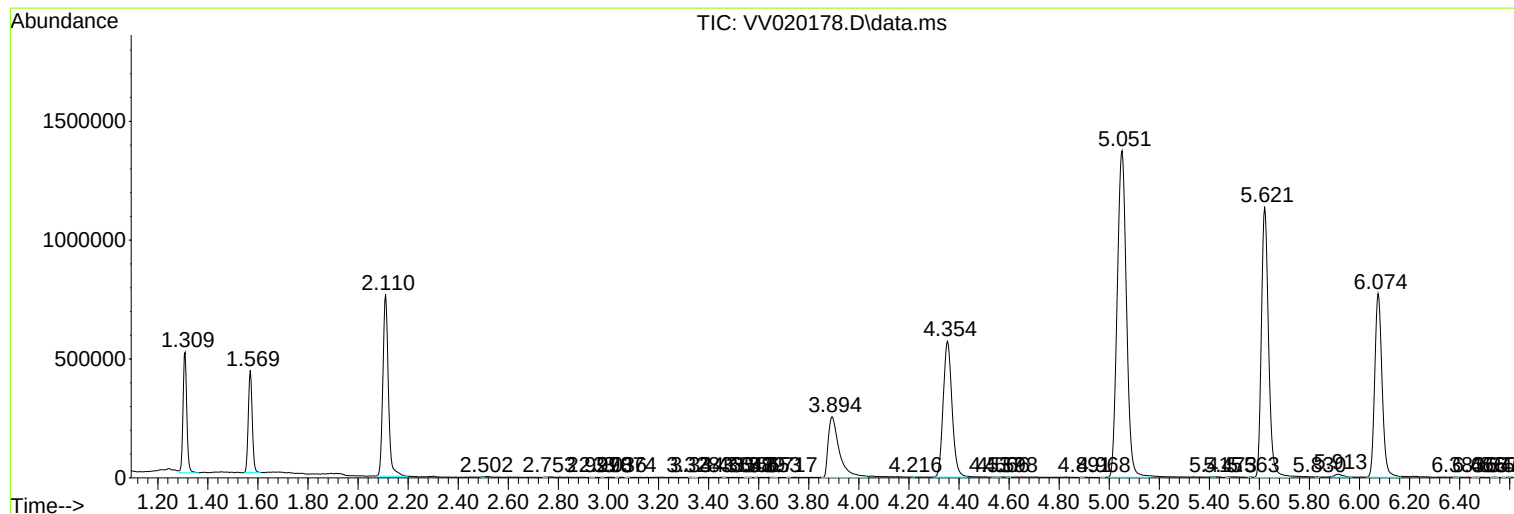

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012721\
Data File : VV020178.D
Acq On : 26 Jan 2021 18:54
Operator : SY/MD
Sample : VV0127WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012721\
Data File : VV020178.D
Acq On : 26 Jan 2021 18:54
Operator : SY/MD
Sample : VV0127WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
