
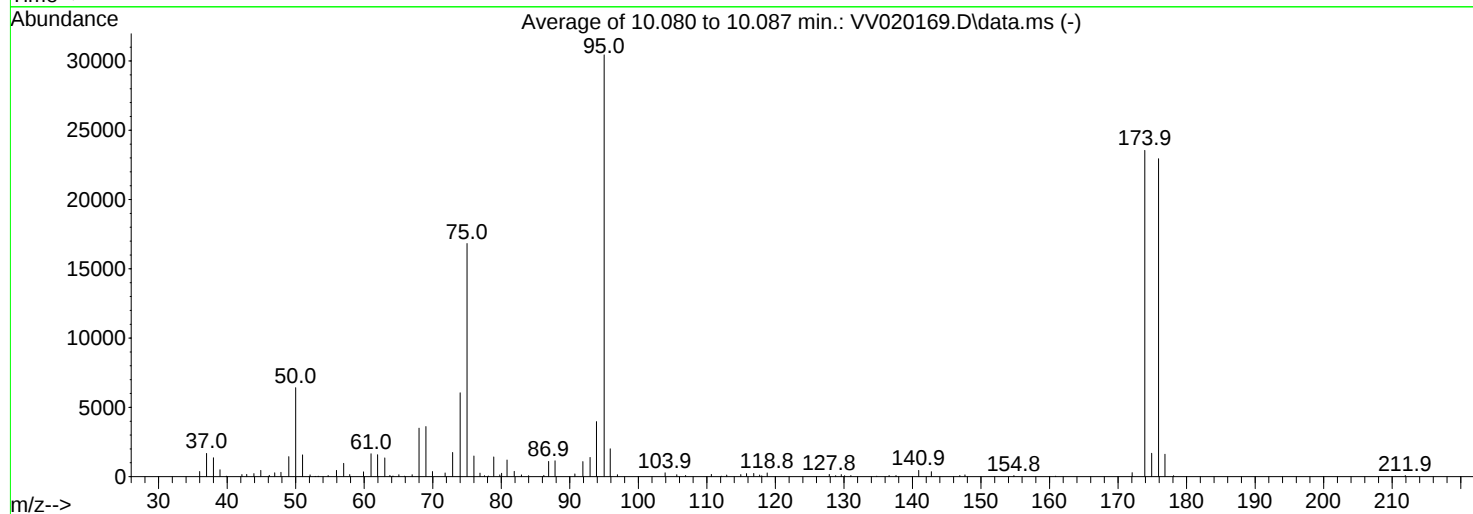


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012721\
 Data File : VV020169.D
 Acq On : 26 Jan 2021 12:20
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB82

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012721WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 27 07:09:38 2021

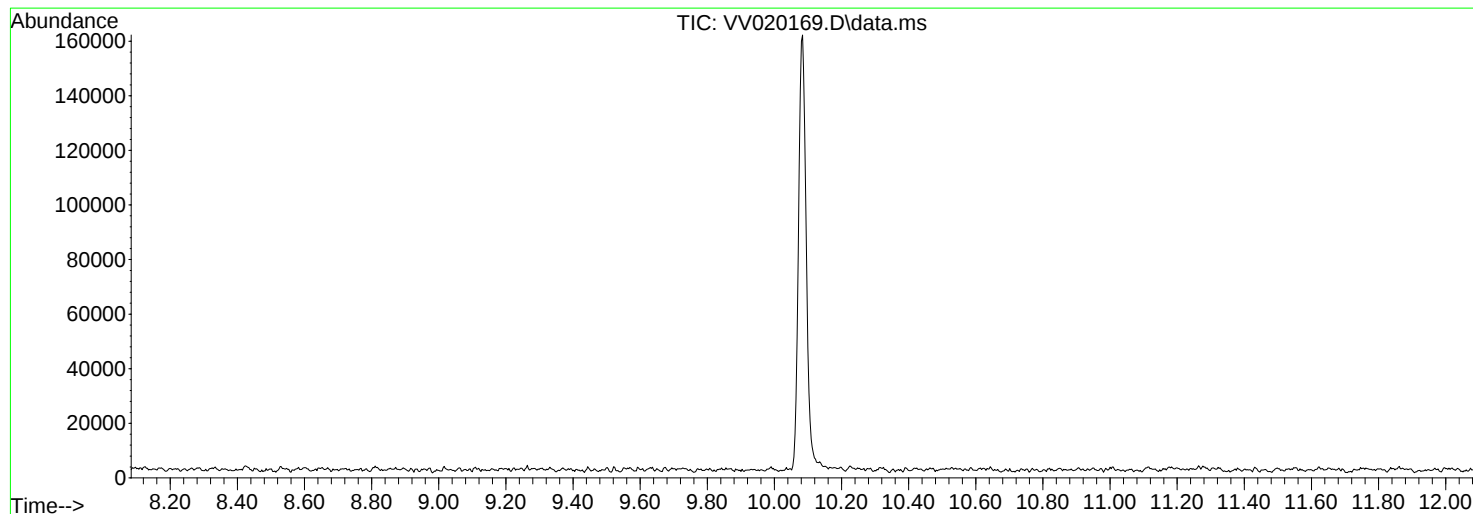

AutoFind: Scans 2796, 2797, 2798; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	6426	PASS
75	95	30	80	55.3	16832	PASS
95	95	100	100	100.0	30445	PASS
96	95	5	9	6.6	2009	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.4	23552	PASS
175	174	5	9	7.2	1684	PASS
176	174	95	101	97.5	22952	PASS
177	176	5	9	7.0	1612	PASS

m/z	Abundance
35.10	131.0
35.60	120.0
36.30	116.0
36.60	143.0
37.70	115.0
38.20	101.0
38.90	151.0
39.80	177.0
40.40	159.0
40.90	130.0
41.80	157.0
42.40	111.0
44.00	215.0
46.80	118.0
47.30	105.0
48.70	113.0
53.00	107.0
54.70	128.0
58.60	117.0
59.60	125.0
61.00	131.0
63.70	109.0
68.20	101.0
77.50	117.0
80.80	145.0
128.30	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	440.0
37.00	1699.0
38.00	1473.0
39.00	720.0
40.00	240.0
40.90	110.0
41.70	150.0
42.10	127.0
42.90	166.0
43.90	415.0
44.90	515.0
47.00	396.0
47.90	298.0
49.00	1423.0
50.00	6433.0
51.00	1623.0
52.00	150.0
52.80	148.0
54.80	199.0
56.00	430.0
57.00	1063.0
57.90	157.0
59.90	329.0
61.00	1805.0
61.90	1615.0
63.00	1317.0
63.80	178.0
64.20	135.0
65.10	158.0
65.90	121.0
66.90	120.0
68.00	3631.0
69.00	3638.0
70.00	336.0
71.80	269.0
72.90	1850.0
74.00	6148.0
75.00	17376.0
76.00	1501.0
76.90	266.0
77.70	130.0
78.10	137.0
78.90	1484.0
79.80	382.0
80.90	1321.0
81.90	384.0
83.10	124.0
84.00	103.0
86.20	140.0
86.90	1086.0
87.90	1205.0
90.70	187.0
91.90	1157.0
93.00	1348.0
93.90	3827.0
95.00	31024.0
95.90	2243.0
97.00	167.0
103.90	250.0
105.60	129.0
110.70	134.0
112.10	105.0
115.00	168.0
115.90	215.0
116.90	230.0
117.70	170.0
118.80	258.0
127.80	147.0
129.60	172.0
130.10	108.0
131.00	138.0
137.60	125.0
140.90	438.0
142.80	388.0
146.90	121.0
147.60	106.0
160.90	100.0
172.10	317.0
173.90	23976.0
174.90	1782.0
175.90	23040.0
176.90	1657.0
211.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	376.0
37.00	1740.0
38.00	1506.0
39.00	650.0
40.00	216.0
40.90	125.0
42.20	155.0
42.80	168.0
43.90	418.0
44.90	472.0
46.10	112.0
47.00	409.0
47.80	328.0
49.00	1514.0
50.00	6645.0
51.00	1604.0
52.10	112.0
52.80	135.0
54.80	234.0
56.00	437.0
57.00	982.0
57.90	156.0
59.90	344.0
61.00	1838.0
61.90	1626.0
63.00	1368.0
63.90	211.0
65.10	135.0
67.00	135.0
68.00	3754.0
69.00	3754.0
70.00	377.0
71.80	288.0
72.90	1813.0
74.00	6209.0
75.00	17344.0
76.00	1499.0
76.90	277.0
77.70	187.0
78.90	1487.0
80.00	354.0
80.90	1405.0
81.90	405.0
82.90	112.0
84.00	102.0
86.20	155.0
86.90	1094.0
87.80	1165.0
90.80	201.0
91.90	1106.0
92.90	1444.0
93.90	4117.0
95.00	31320.0
95.90	2068.0
96.90	150.0
103.90	282.0
105.60	144.0
106.90	102.0
110.60	176.0
112.90	164.0
115.00	154.0
115.80	224.0
116.90	229.0
117.70	167.0
118.80	271.0
127.80	167.0
128.80	107.0
129.60	153.0
130.10	102.0
131.00	115.0
134.80	104.0
136.60	128.0
137.60	126.0
140.90	478.0
142.70	372.0
146.90	111.0
147.60	125.0
154.80	106.0
172.10	289.0
173.90	24272.0
174.90	1670.0
175.90	23704.0
176.80	1665.0
178.10	102.0
211.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	292.0
37.00	1589.0
38.00	1427.0
39.00	577.0
40.00	186.0
40.90	129.0
42.20	156.0
42.80	149.0
43.90	485.0
44.90	362.0
46.20	155.0
47.00	373.0
47.80	309.0
49.00	1409.0
50.00	6199.0
51.00	1501.0
52.20	113.0
52.80	111.0
53.30	113.0
54.80	201.0
55.90	479.0
57.00	848.0
57.90	150.0
59.90	366.0
61.00	1698.0
62.00	1512.0
63.00	1375.0
63.90	210.0
65.00	136.0
67.10	163.0
68.00	3401.0
69.00	3465.0
69.90	409.0
71.80	247.0
72.90	1563.0
74.00	5785.0
75.00	15775.0
76.00	1468.0
76.90	227.0
77.60	231.0
78.90	1286.0
80.10	359.0
80.90	1320.0
81.90	369.0
82.80	134.0
86.90	1128.0
87.80	1045.0
90.80	215.0
91.90	998.0
92.90	1370.0
93.90	3967.0
95.00	28992.0
95.90	1717.0
96.90	114.0
103.90	291.0
105.60	151.0
106.90	127.0
110.60	173.0
112.90	187.0
114.90	113.0
115.70	214.0
116.80	226.0
118.00	187.0
118.80	278.0
127.90	162.0
128.80	104.0
129.60	114.0
136.60	116.0
140.90	446.0
142.70	325.0
147.70	139.0
154.80	142.0
172.00	251.0
173.90	22408.0
174.90	1599.0
175.90	22112.0
176.90	1514.0
178.10	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82