

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012722\
 Data File : VW024453.D
 Acq On : 27 Jan 2022 15:50
 Operator : SY/MD
 Sample : VW0127WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK297

Quant Time: Jan 28 03:21:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 28 03:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	147783	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	156983	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	78275	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	57232	4.420	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.400%	
7) Chloroethane-d5	1.568	69	54405	4.817	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.400%	
11) 1,1-Dichloroethene-d2	2.108	63	89498	3.617	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.400%	
20) 2-Butanone-d5	3.912	46	77287	37.455	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	74.900%	
24) Chloroform-d	4.346	84	122157	4.972	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.400%	
26) 1,2-Dichloroethane-d4	5.030	65	58094	5.221	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.400%	
32) Benzene-d6	5.043	84	230408	4.914	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.200%	
36) 1,2-Dichloropropane-d6	6.066	67	73640	4.988	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.800%	
41) Toluene-d8	7.313	98	189854	4.413	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.200%	
43) trans-1,3-Dichloroprop...	7.622	79	24267	4.787	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.800%	
46) 2-Hexanone-d5	8.088	63	84088	48.509	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.020%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	45459	5.173	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	71433	5.322	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.400%	
Target Compounds					Qvalue	
25) Chloroform	4.375	83	4457	0.198	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024453.D
Acq On : 27 Jan 2022 15:50
Operator : SY/MD
Sample : VV0127WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK297

Quant Time: Jan 28 03:21:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 28 03:20:33 2022
Response via : Initial Calibration

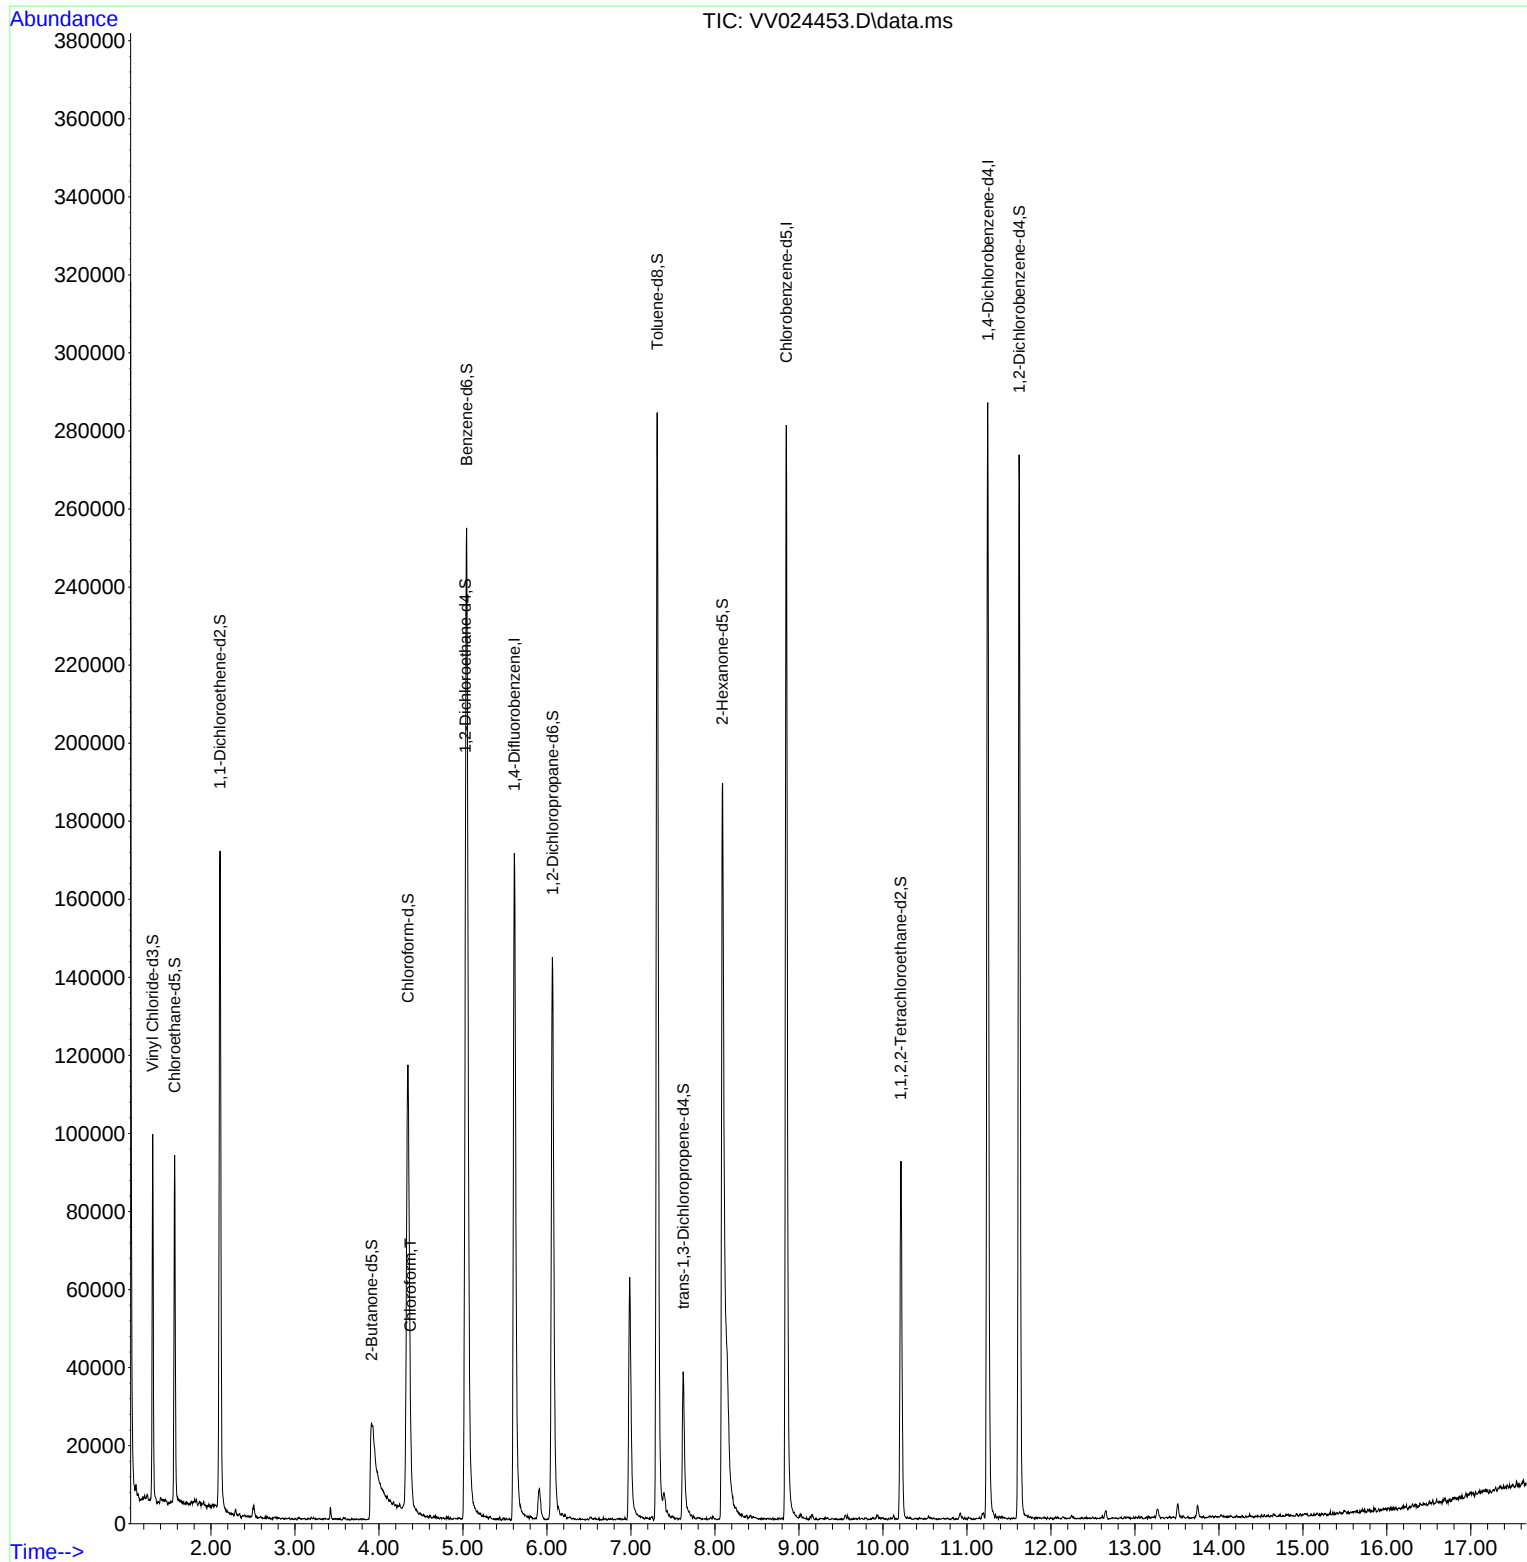

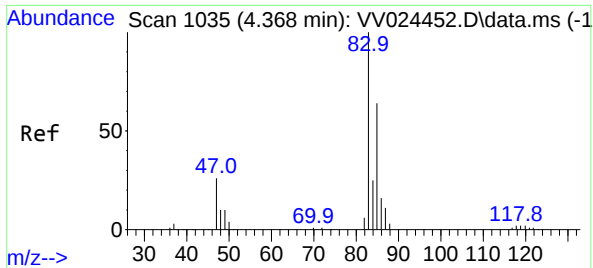

#25
 Chloroform
 Concen: 0.198 ug/L
 RT: 4.375 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV024453.D
 Acq: 27 Jan 2022 15:50

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK297

Tgt Ion: 83 Resp: 4457

Ion	Ratio	Lower	Upper
83	100		
85	73.7	45.2	84.0

