

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024454.D
 Acq On : 27 Jan 2022 16:13
 Operator : SY/MD
 Sample : N1275-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F51

Quant Time: Jan 28 03:21:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 28 03:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	147885	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	157024	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77371	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	54852	4.234	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.600%
7) Chloroethane-d5	1.571	69	52460	4.642	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.800%
11) 1,1-Dichloroethene-d2	2.111	63	86001	3.473	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.400%
20) 2-Butanone-d5	3.905	46	115942	56.149	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.300%
24) Chloroform-d	4.349	84	119630	4.866	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
26) 1,2-Dichloroethane-d4	5.034	65	58313	5.237	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.800%
32) Benzene-d6	5.053	84	224589	4.789	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
36) 1,2-Dichloropropane-d6	6.069	67	71819	4.863	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.200%
41) Toluene-d8	7.317	98	189819	4.411	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	7.625	79	22640	4.465	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.092	63	79912	46.087	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.180%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40963	4.660	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	70865	5.341	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.800%
Target Compounds					Qvalue	
13) Acetone	2.188	43	10275	9.545	ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024454.D
Acq On : 27 Jan 2022 16:13
Operator : SY/MD
Sample : N1275-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F51

Quant Time: Jan 28 03:21:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 28 03:20:33 2022
Response via : Initial Calibration

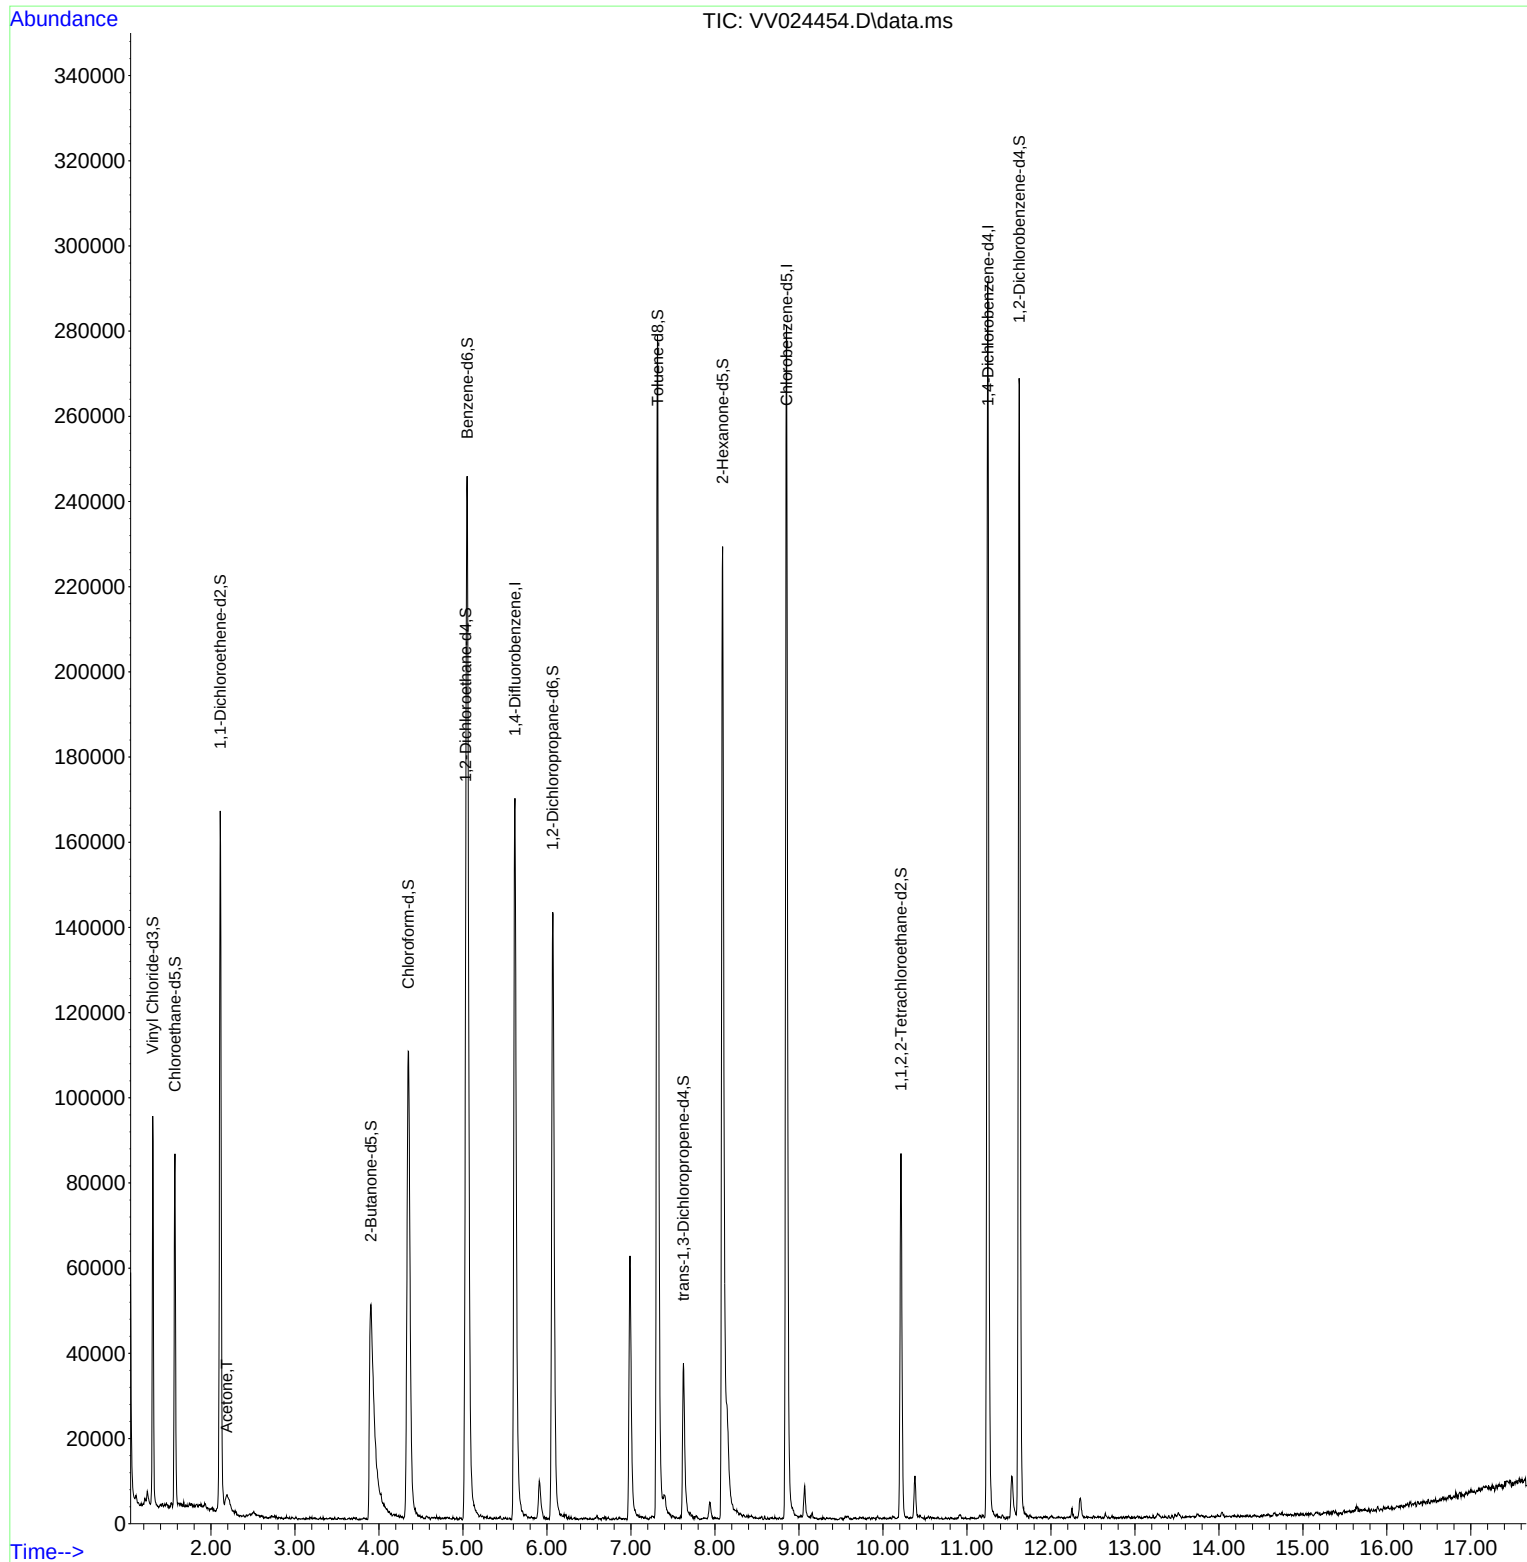

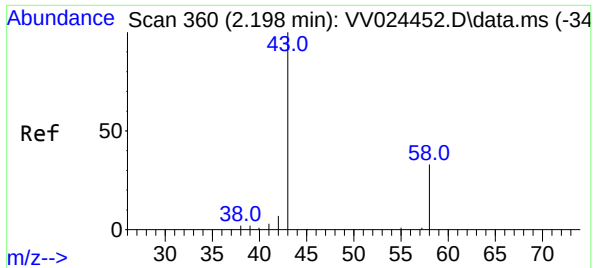

#13
 Acetone
 Concen: 9.545 ug/L
 RT: 2.188 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV024454.D
 Acq: 27 Jan 2022 16:13

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F51

Tgt Ion: 43 Resp: 10275
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 41.4

