

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024455.D
 Acq On : 27 Jan 2022 16:36
 Operator : SY/MD
 Sample : N1275-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F52

Quant Time: Jan 28 03:21:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 28 03:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	150858	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	160184	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79553	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	55437	4.195	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.800%
7) Chloroethane-d5	1.571	69	52866	4.586	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.800%
11) 1,1-Dichloroethene-d2	2.111	63	87188	3.451	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.000%
20) 2-Butanone-d5	3.899	46	126510	60.060	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.120%
24) Chloroform-d	4.352	84	121825	4.858	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.034	65	60095	5.291	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%
32) Benzene-d6	5.050	84	226745	4.740	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	6.069	67	73213	4.860	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.200%
41) Toluene-d8	7.317	98	191776	4.369	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.625	79	23380	4.520	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%
46) 2-Hexanone-d5	8.088	63	82602	46.699	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.400%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42611	4.752	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	72684	5.328	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.600%
Target Compounds					Qvalue	
13) Acetone	2.185	43	9726	8.857	ug/L	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024455.D
Acq On : 27 Jan 2022 16:36
Operator : SY/MD
Sample : N1275-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F52

Quant Time: Jan 28 03:21:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 28 03:20:33 2022
Response via : Initial Calibration

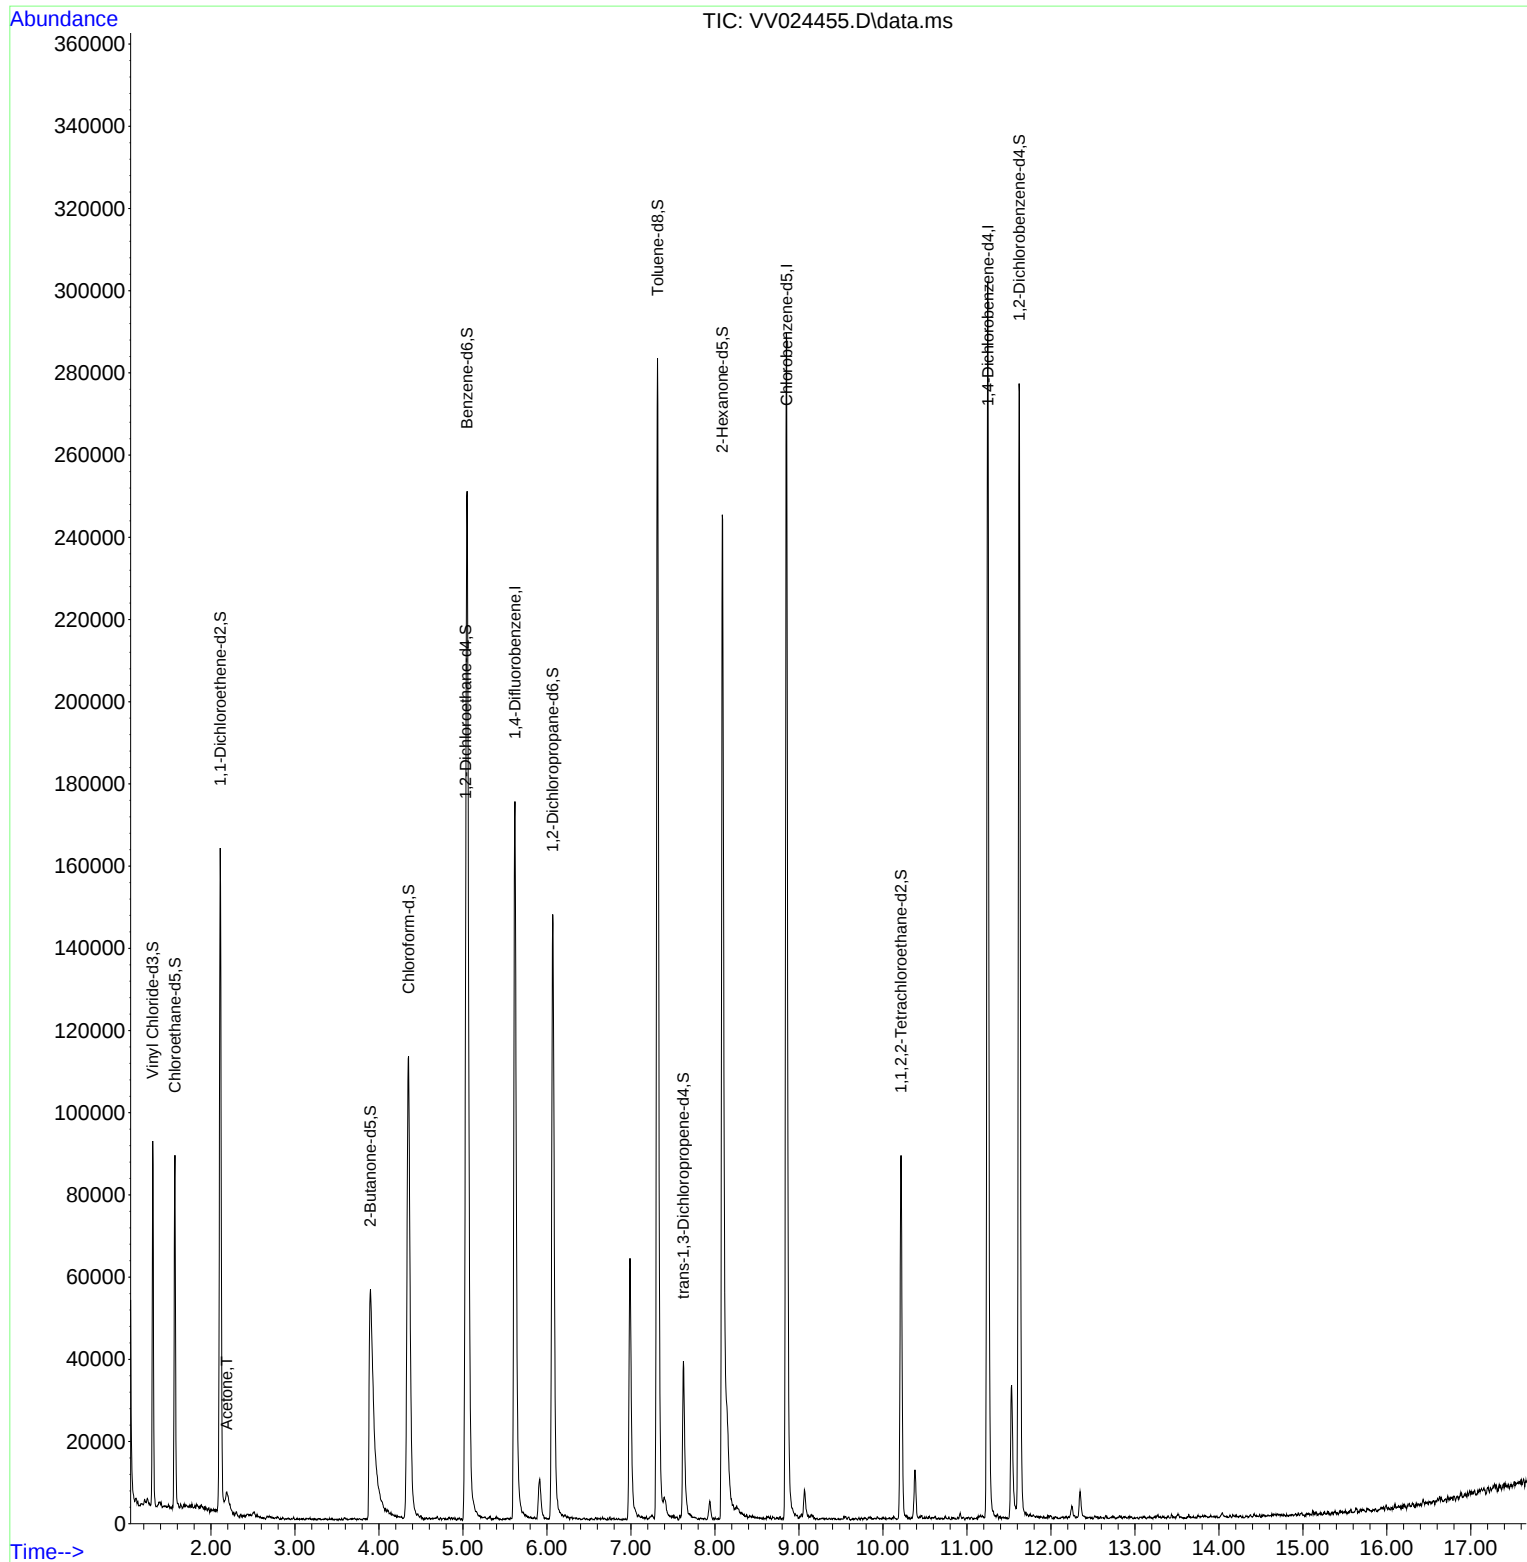

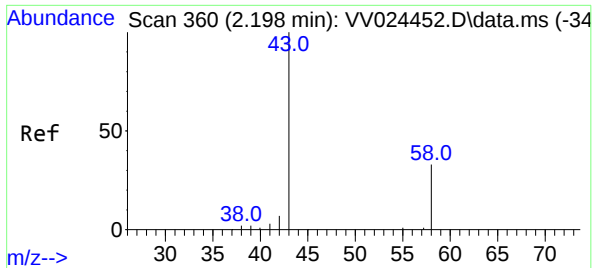

#13
Acetone
Concen: 8.857 ug/L
RT: 2.185 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV024455.D
Acq: 27 Jan 2022 16:36

Instrument :
MSVOA_V
ClientSampleId :
C0F52

Tgt Ion: 43 Resp: 9726
Ion Ratio Lower Upper
43 100
58 38.4 0.0 41.4

