

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024456.D
 Acq On : 27 Jan 2022 17:00
 Operator : SY/MD
 Sample : N1275-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jan 28 03:21:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 28 03:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	144985	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	153098	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76033	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	55958	4.406	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.200%
7) Chloroethane-d5	1.568	69	54014	4.875	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.400%
11) 1,1-Dichloroethene-d2	2.111	63	87234	3.593	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.800%
20) 2-Butanone-d5	3.905	46	126258	62.368	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.740%
24) Chloroform-d	4.349	84	119965	4.977	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
26) 1,2-Dichloroethane-d4	5.034	65	58188	5.330	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	5.050	84	221354	4.841	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	6.069	67	74796	5.195	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.800%
41) Toluene-d8	7.317	98	184586	4.400	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
43) trans-1,3-Dichloroprop...	7.625	79	23187	4.690	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.800%
46) 2-Hexanone-d5	8.092	63	82863	49.015	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43026	5.021	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	68554	5.258	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds					Qvalue	
25) Chloroform	4.384	83	4599	0.208	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024456.D
Acq On : 27 Jan 2022 17:00
Operator : SY/MD
Sample : N1275-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jan 28 03:21:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 28 03:20:33 2022
Response via : Initial Calibration

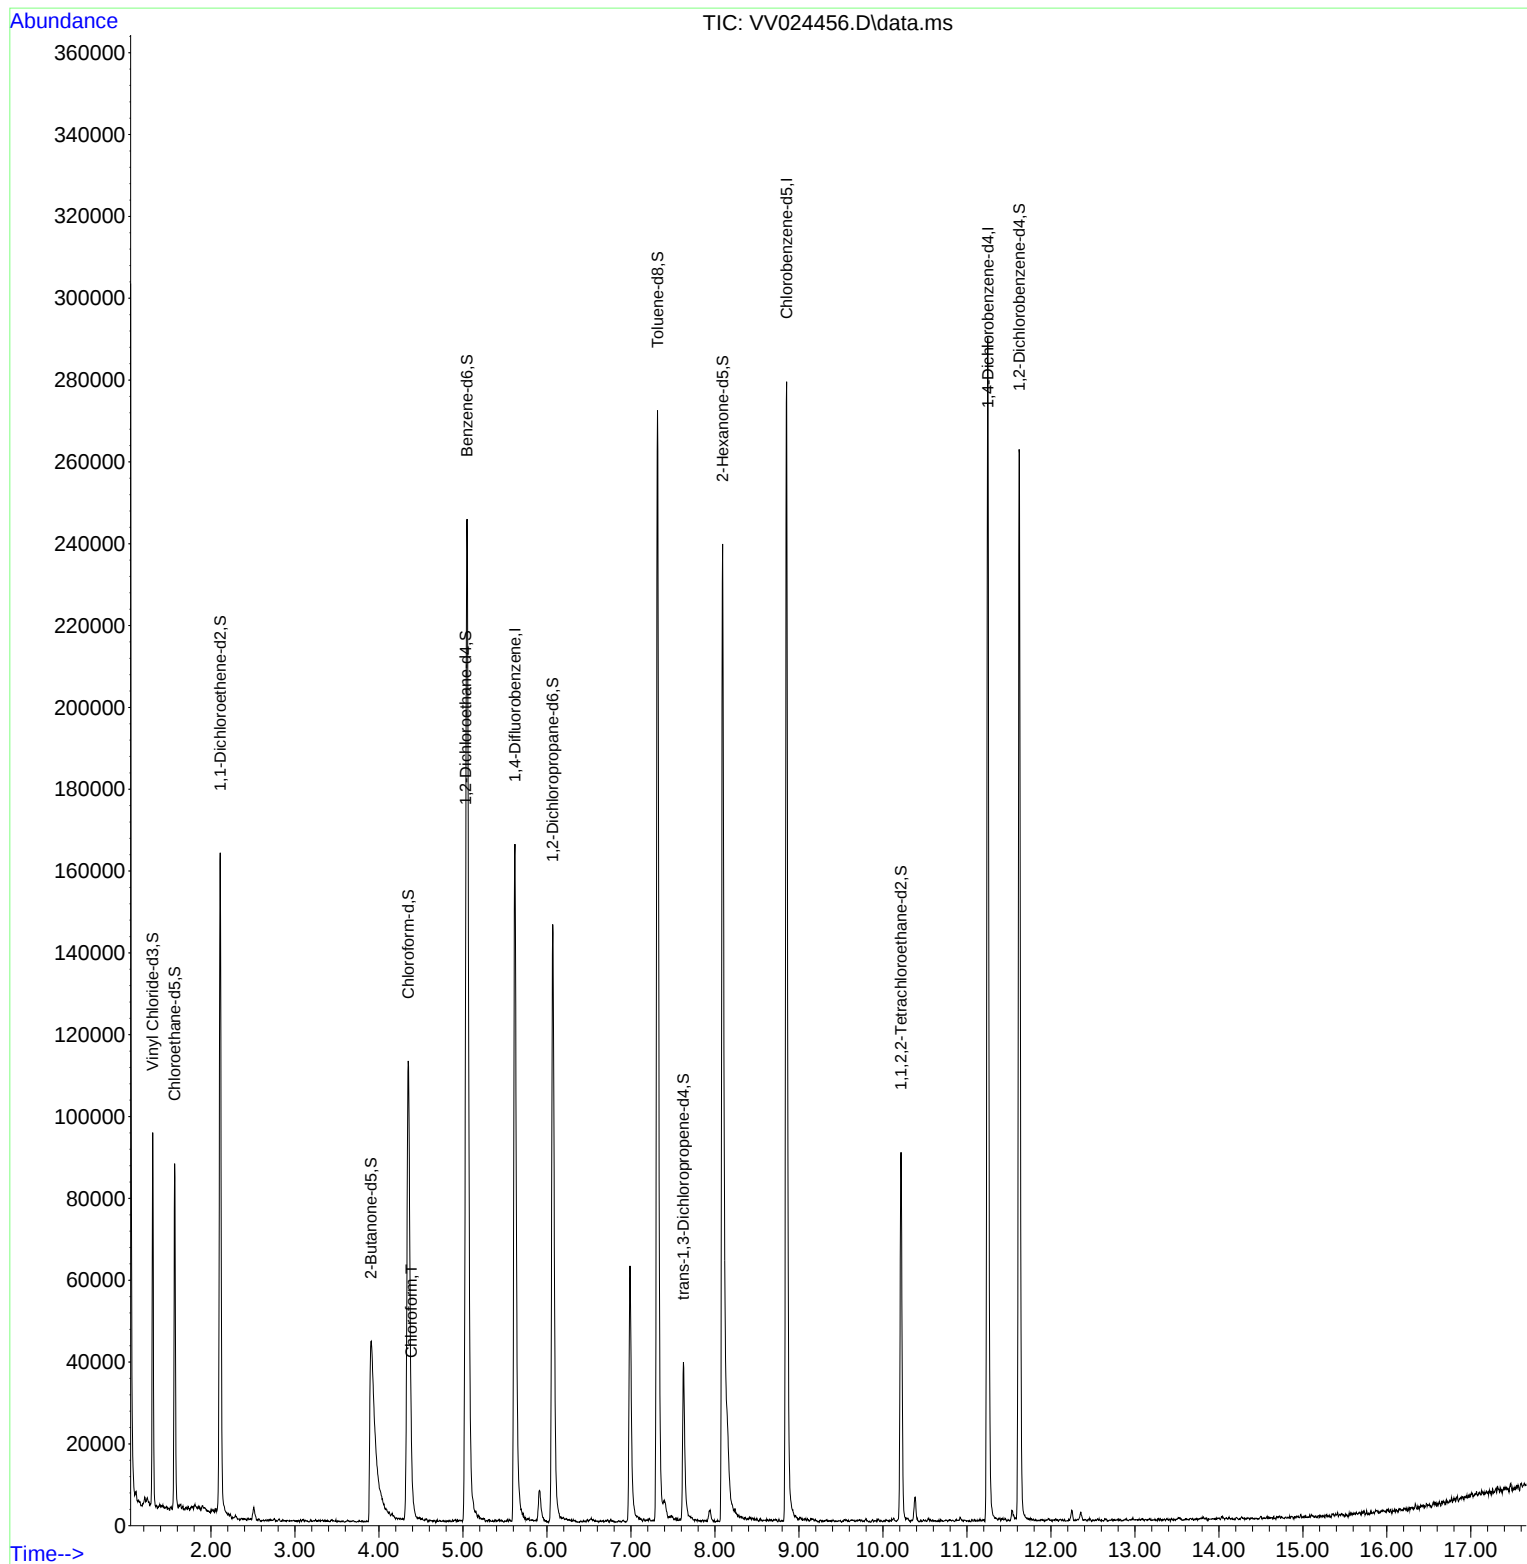

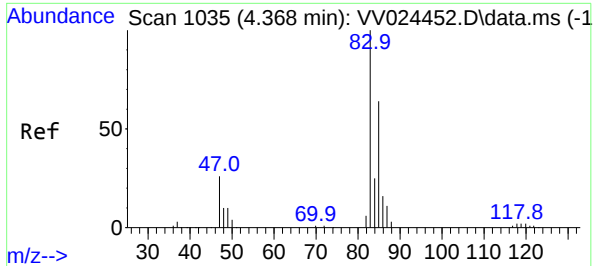

#25
Chloroform
Concen: 0.208 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.016 min
Lab File: VV024456.D
Acq: 27 Jan 2022 17:00

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 83 Resp: 4599
Ion Ratio Lower Upper
83 100
85 68.1 45.2 84.0

