

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024458.D
 Acq On : 27 Jan 2022 17:46
 Operator : SY/MD
 Sample : N1317-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA1

Quant Time: Jan 28 03:22:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 28 03:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	138503	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	149430	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75275	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	53915	4.443	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.800%
7) Chloroethane-d5	1.568	69	50903	4.809	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.200%
11) 1,1-Dichloroethene-d2	2.108	63	83809	3.614	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.200%
20) 2-Butanone-d5	3.912	46	87781	45.391	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.780%
24) Chloroform-d	4.349	84	117778	5.115	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
26) 1,2-Dichloroethane-d4	5.037	65	57046	5.470	ug/L	0.01
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.400%
32) Benzene-d6	5.053	84	217002	4.862	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
36) 1,2-Dichloropropane-d6	6.069	67	71098	5.059	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.317	98	183223	4.475	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.400%
43) trans-1,3-Dichloroprop...	7.625	79	24841	5.148	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.000%
46) 2-Hexanone-d5	8.092	63	93191	56.477	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45425	5.431	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	70291	5.446	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.000%
Target Compounds						
					Qvalue	
13) Acetone	2.201	43	6663	6.609	ug/L	72
42) Toluene	7.387	91	912620	21.543	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024458.D
Acq On : 27 Jan 2022 17:46
Operator : SY/MD
Sample : N1317-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA1

Quant Time: Jan 28 03:22:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 28 03:20:33 2022
Response via : Initial Calibration




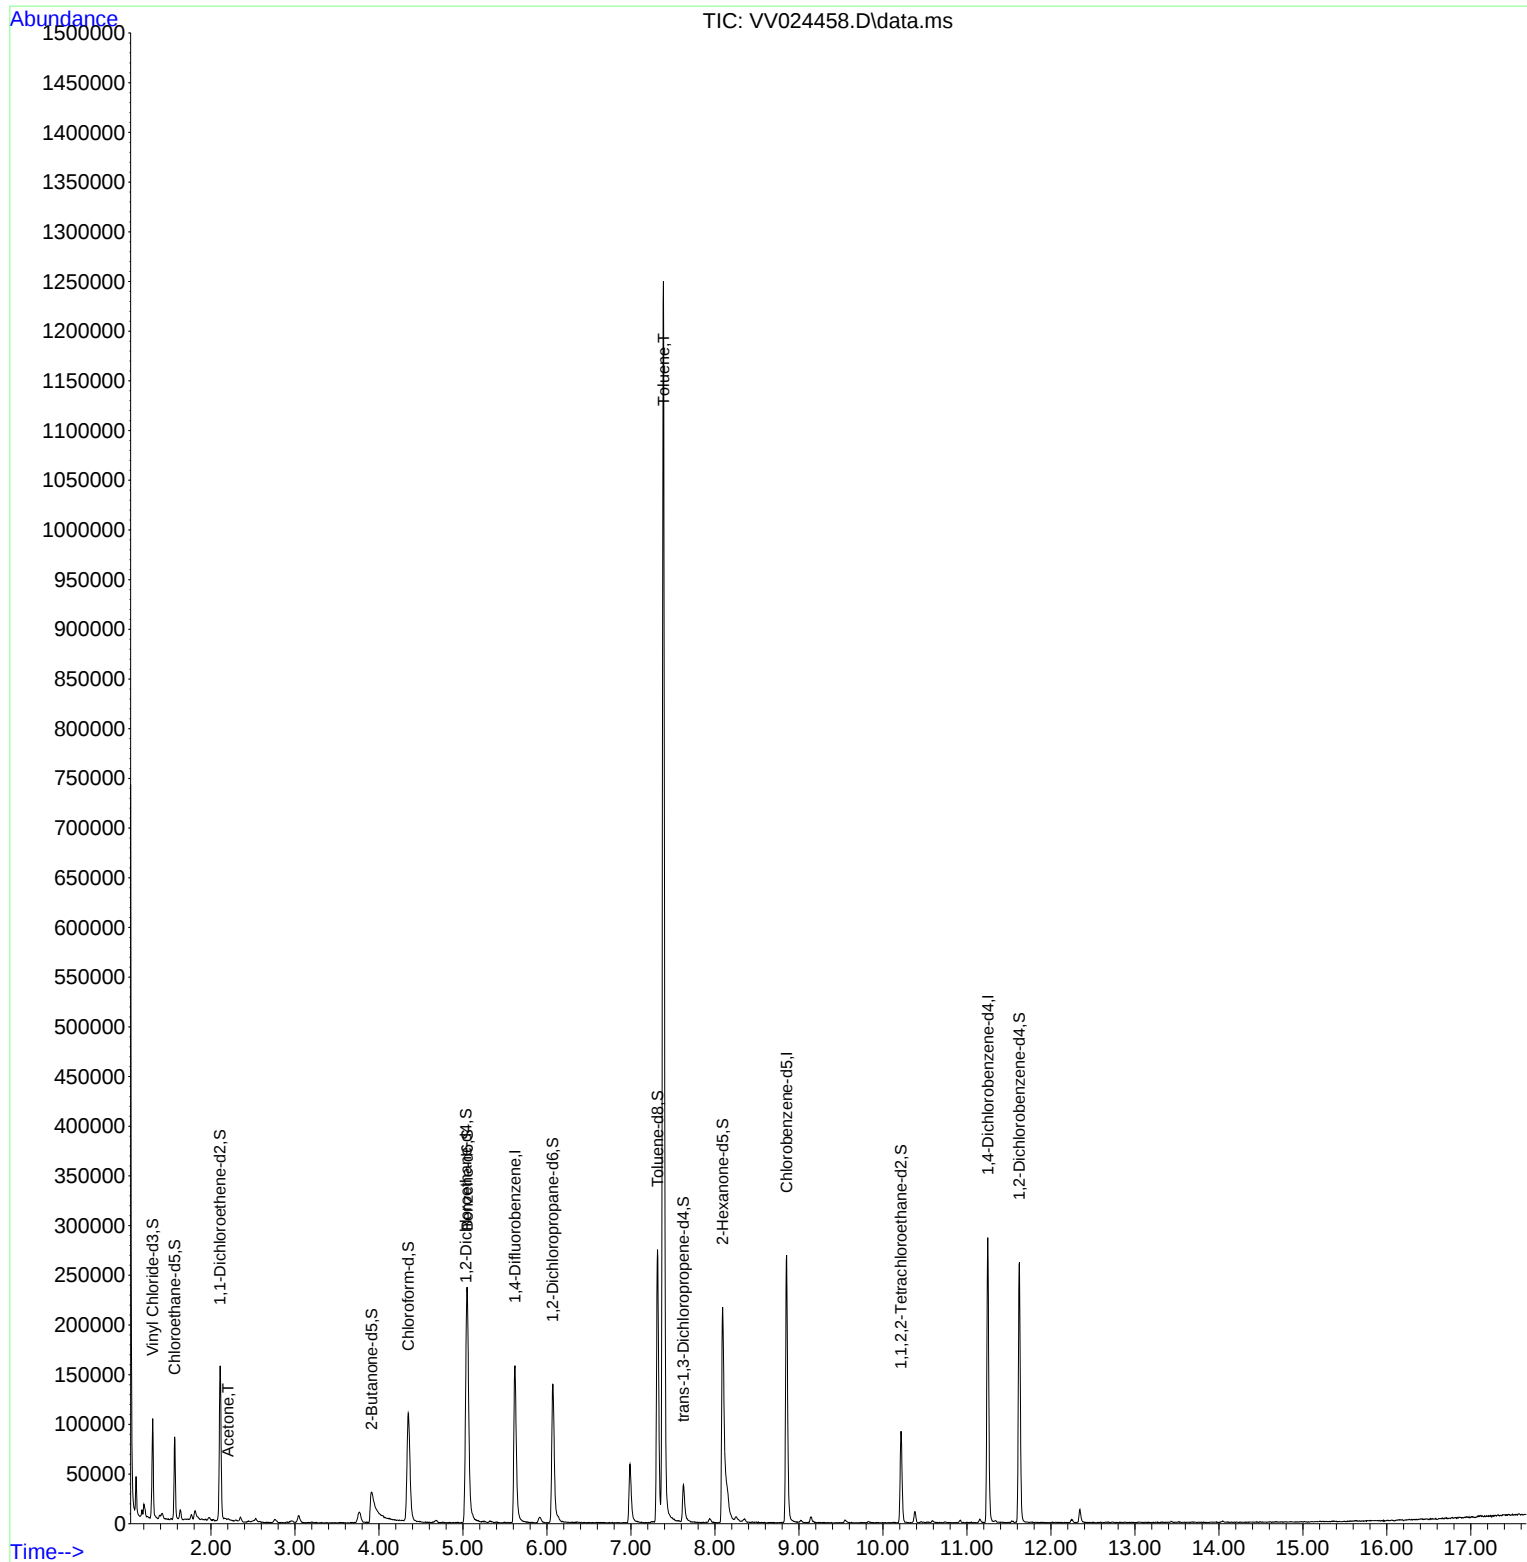


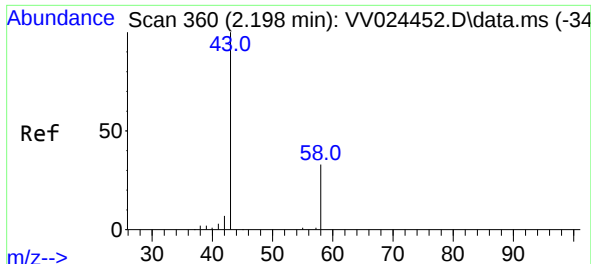

#13
Acetone
Concen: 6.609 ug/L
RT: 2.201 min Scan# 361
Delta R.T. 0.003 min
Lab File: VV024458.D
Acq: 27 Jan 2022 17:46

Instrument :
MSVOA_V
ClientSampleId :
H0AA1

Tgt Ion: 43 Resp: 6663
Ion Ratio Lower Upper
43 100
58 33.9 0.0 41.4

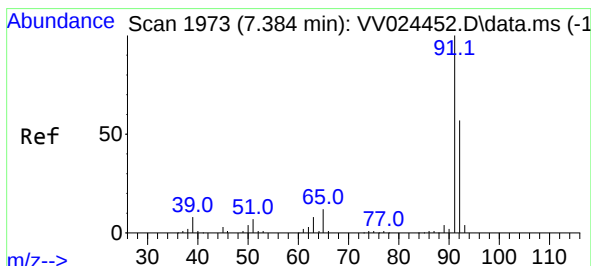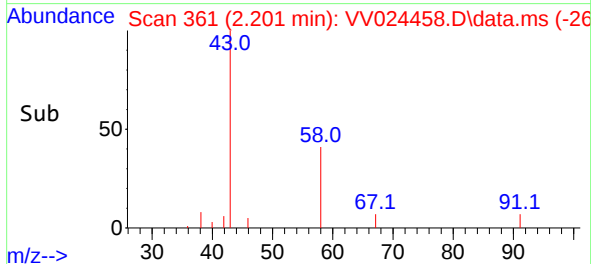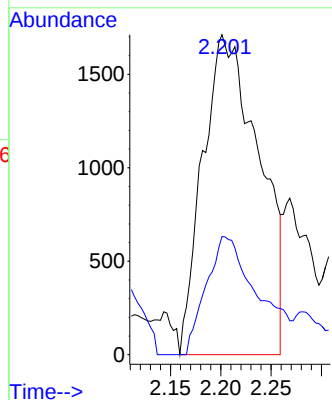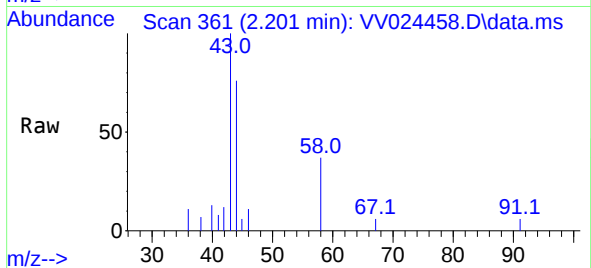

#42
Toluene
Concen: 21.543 ug/L
RT: 7.387 min Scan# 1974
Delta R.T. 0.003 min
Lab File: VV024458.D
Acq: 27 Jan 2022 17:46

Tgt Ion: 91 Resp: 912620
Ion Ratio Lower Upper
91 100
92 57.3 41.5 77.1

