

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012722\
 Data File : VW024460.D
 Acq On : 27 Jan 2022 18:32
 Operator : SY/MD
 Sample : N1317-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA3

Quant Time: Jan 28 03:22:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 28 03:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	141426	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	150860	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76753	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	52112	4.206	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.200%
7) Chloroethane-d5	1.571	69	51299	4.746	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.000%
11) 1,1-Dichloroethene-d2	2.111	63	80212	3.387	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.800%
20) 2-Butanone-d5	3.896	46	113984	57.722	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.440%
24) Chloroform-d	4.349	84	116655	4.962	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
26) 1,2-Dichloroethane-d4	5.034	65	57049	5.358	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
32) Benzene-d6	5.053	84	214142	4.753	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
36) 1,2-Dichloropropane-d6	6.069	67	71385	5.031	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.600%
41) Toluene-d8	7.317	98	180787	4.373	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.625	79	24174	4.962	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.200%
46) 2-Hexanone-d5	8.088	63	87519	52.537	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.080%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44228	5.237	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	67811	5.152	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds					Qvalue	
13) Acetone	2.191	43	10242	9.949	ug/L	75
42) Toluene	7.387	91	1691048	39.540	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024460.D
Acq On : 27 Jan 2022 18:32
Operator : SY/MD
Sample : N1317-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA3

Quant Time: Jan 28 03:22:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 28 03:20:33 2022
Response via : Initial Calibration




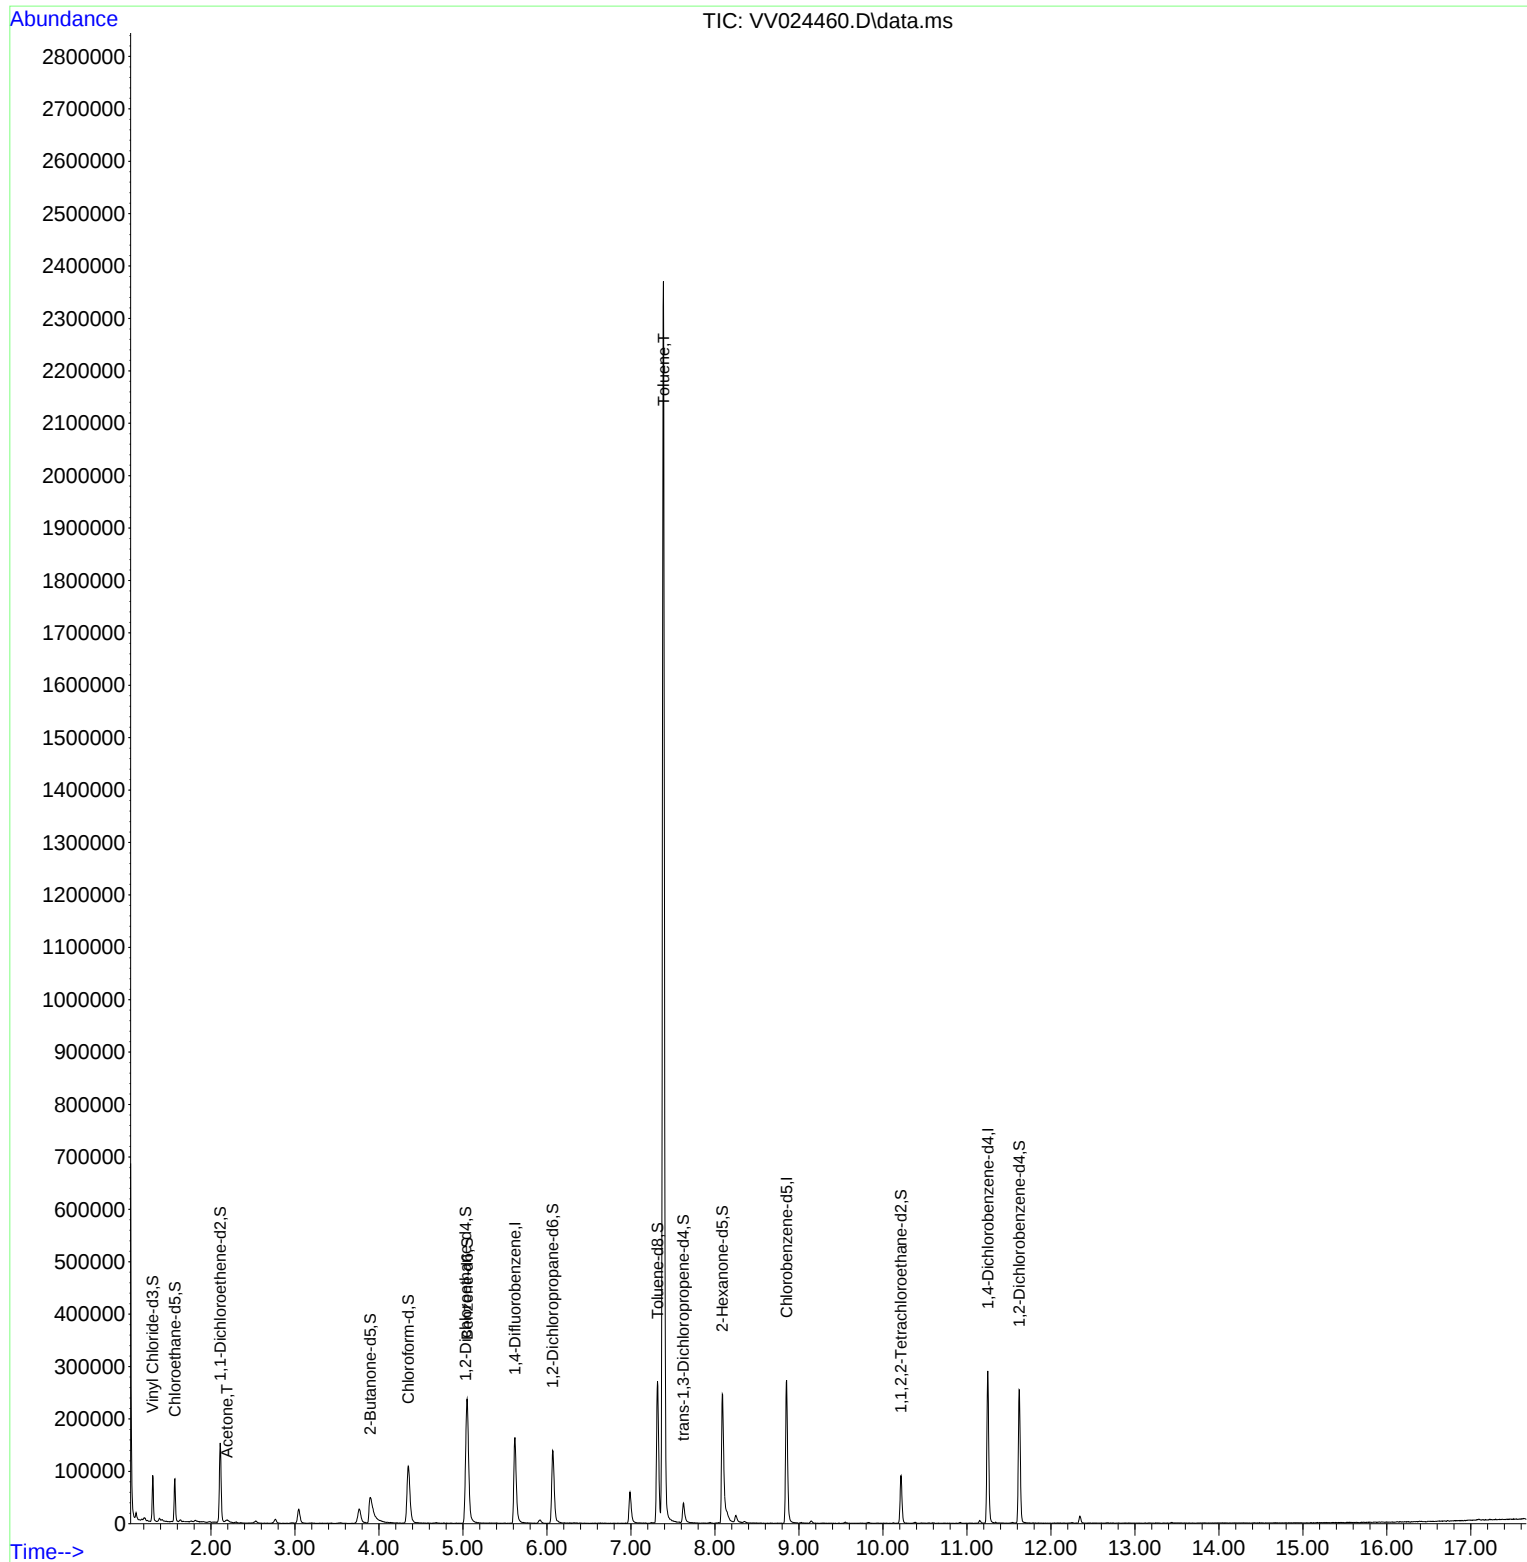


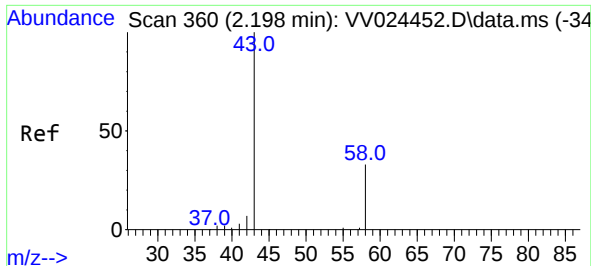

#13
Acetone
Concen: 9.949 ug/L
RT: 2.191 min Scan# 31
Delta R.T. -0.006 min
Lab File: VV024460.D
Acq: 27 Jan 2022 18:32

Instrument :
MSVOA_V
ClientSampleId :
H0AA3

Tgt Ion: 43 Resp: 10242
Ion Ratio Lower Upper
43 100
58 32.3 0.0 41.4

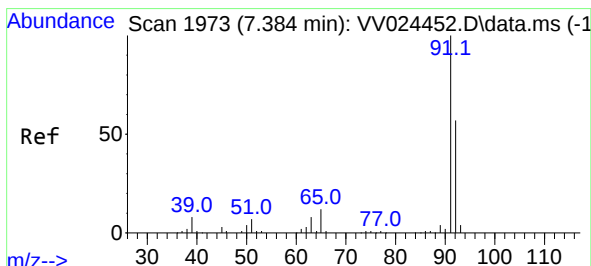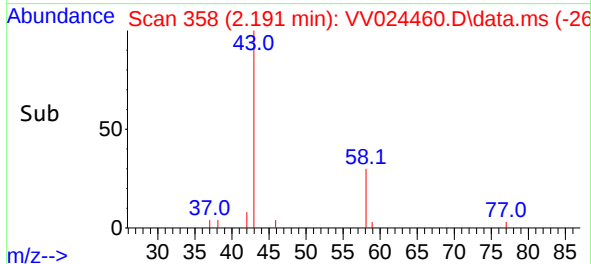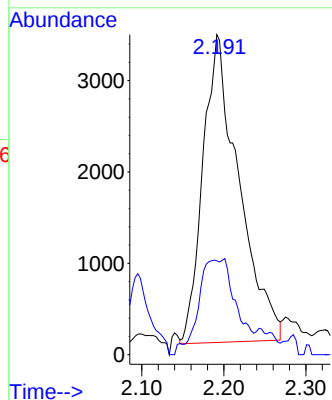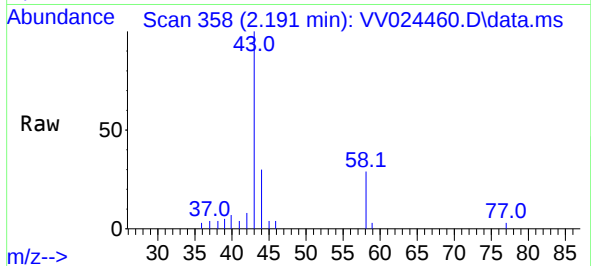

#42
Toluene
Concen: 39.540 ug/L
RT: 7.387 min Scan# 1974
Delta R.T. 0.003 min
Lab File: VV024460.D
Acq: 27 Jan 2022 18:32

Tgt Ion: 91 Resp: 1691048
Ion Ratio Lower Upper
91 100
92 58.1 41.5 77.1

