

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024466.D
 Acq On : 27 Jan 2022 20:52
 Operator : SY/MD
 Sample : N1317-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AB0

Quant Time: Jan 28 03:23:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 28 03:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	139052	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150806	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	74899	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	53015	4.352	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.000%
7) Chloroethane-d5	1.568	69	52299	4.921	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.400%
11) 1,1-Dichloroethene-d2	2.108	63	84598	3.633	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	3.915	46	97007	49.963	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.920%
24) Chloroform-d	4.349	84	119770	5.181	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.600%
26) 1,2-Dichloroethane-d4	5.034	65	58415	5.579	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.600%
32) Benzene-d6	5.053	84	219687	4.878	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	6.069	67	71776	5.061	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.317	98	180516	4.368	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.625	79	21729	4.462	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.091	63	89514	53.754	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.500%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46705	5.533	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	69822	5.436	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.800%
Target Compounds						Qvalue
34) Trichloroethene	5.928	95	2611	0.229	ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024466.D
Acq On : 27 Jan 2022 20:52
Operator : SY/MD
Sample : N1317-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB0


Quant Time: Jan 28 03:23:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 28 03:20:33 2022
Response via : Initial Calibration

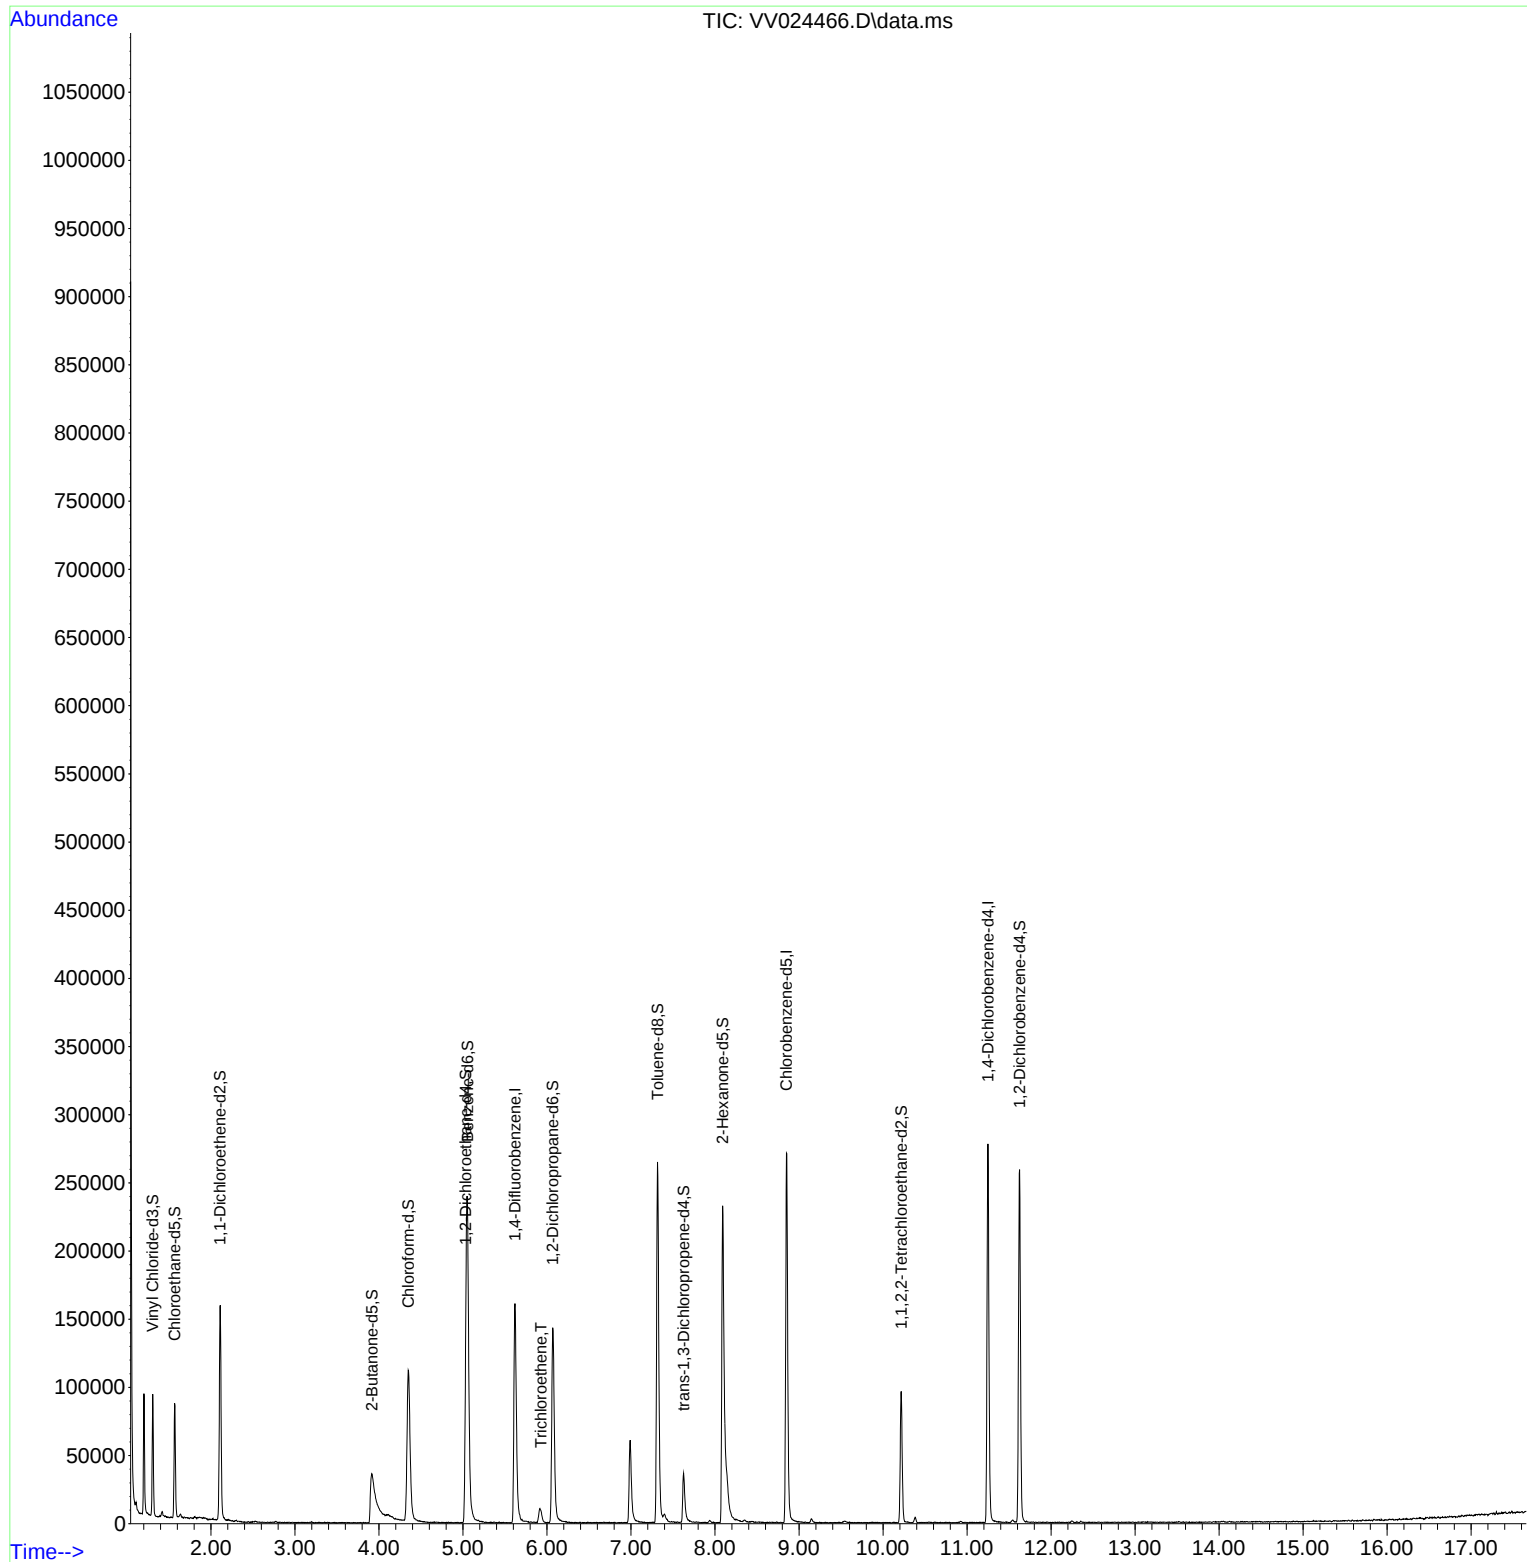

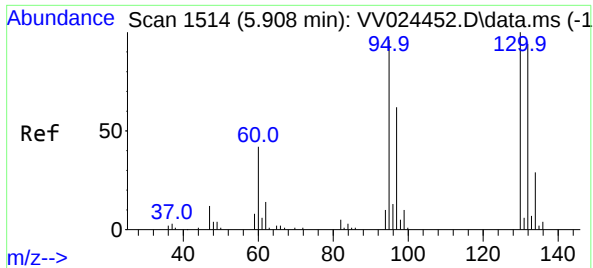

#34
 Trichloroethene
 Concen: 0.229 ug/L
 RT: 5.928 min Scan# 11
 Delta R.T. 0.019 min
 Lab File: VV024466.D
 Acq: 27 Jan 2022 20:52

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AB0

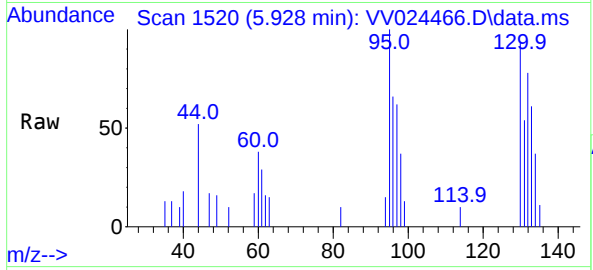

Tgt Ion: 95 Resp: 2611

Ion	Ratio	Lower	Upper
95	100		
97	62.3	45.2	84.0
132	78.0	76.1	141.3
130	92.7	75.4	140.0

