

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024454.D
 Acq On : 27 Jan 2022 16:13
 Operator : SY/MD
 Sample : N1275-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F51

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	91250	89667	14.25%	1.815%
2	1.571	157	165	175	rBV	82619	93821	14.91%	1.899%
3	2.111	317	333	349	rBV	164397	240008	38.14%	4.859%
4	2.192	349	358	370	rVB3	2502	6904	1.10%	0.140%
5	3.905	878	891	926	rBV	50505	203026	32.26%	4.110%
6	4.349	1011	1029	1054	rBV	109743	284806	45.26%	5.766%
7	5.050	1229	1247	1278	rBV2	245062	629278	100.00%	12.739%
8	5.619	1411	1424	1450	rBV	169428	355095	56.43%	7.188%
9	5.908	1503	1514	1530	rBV4	8802	18152	2.88%	0.367%
10	6.069	1551	1564	1593	rBV	142613	304565	48.40%	6.166%
11	6.989	1839	1850	1867	rBV2	61989	116868	18.57%	2.366%
12	7.317	1940	1952	1970	rBV	277679	489314	77.76%	9.906%
13	7.625	2039	2048	2070	rBV	36313	67869	10.79%	1.374%
14	7.940	2137	2146	2155	rBV4	3865	6361	1.01%	0.129%
15	8.092	2181	2193	2229	rBV	228303	492788	78.31%	9.976%
16	8.854	2418	2430	2450	rBV	280206	469520	74.61%	9.505%
17	9.069	2487	2497	2512	rBV2	7407	11053	1.76%	0.224%
18	10.217	2843	2854	2870	rBV	85444	135248	21.49%	2.738%
19	10.381	2895	2905	2916	rBV	9891	15061	2.39%	0.305%
20	11.249	3162	3175	3193	rBV	290274	458776	72.91%	9.287%
21	11.535	3256	3264	3280	rBV3	9735	19151	3.04%	0.388%
22	11.622	3280	3291	3307	rBV	266889	424264	67.42%	8.589%
23	12.352	3508	3518	3530	rVB6	4595	8211	1.30%	0.166%


Sum of corrected areas: 4939806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024454.D
Acq On : 27 Jan 2022 16:13
Operator : SY/MD
Sample : N1275-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

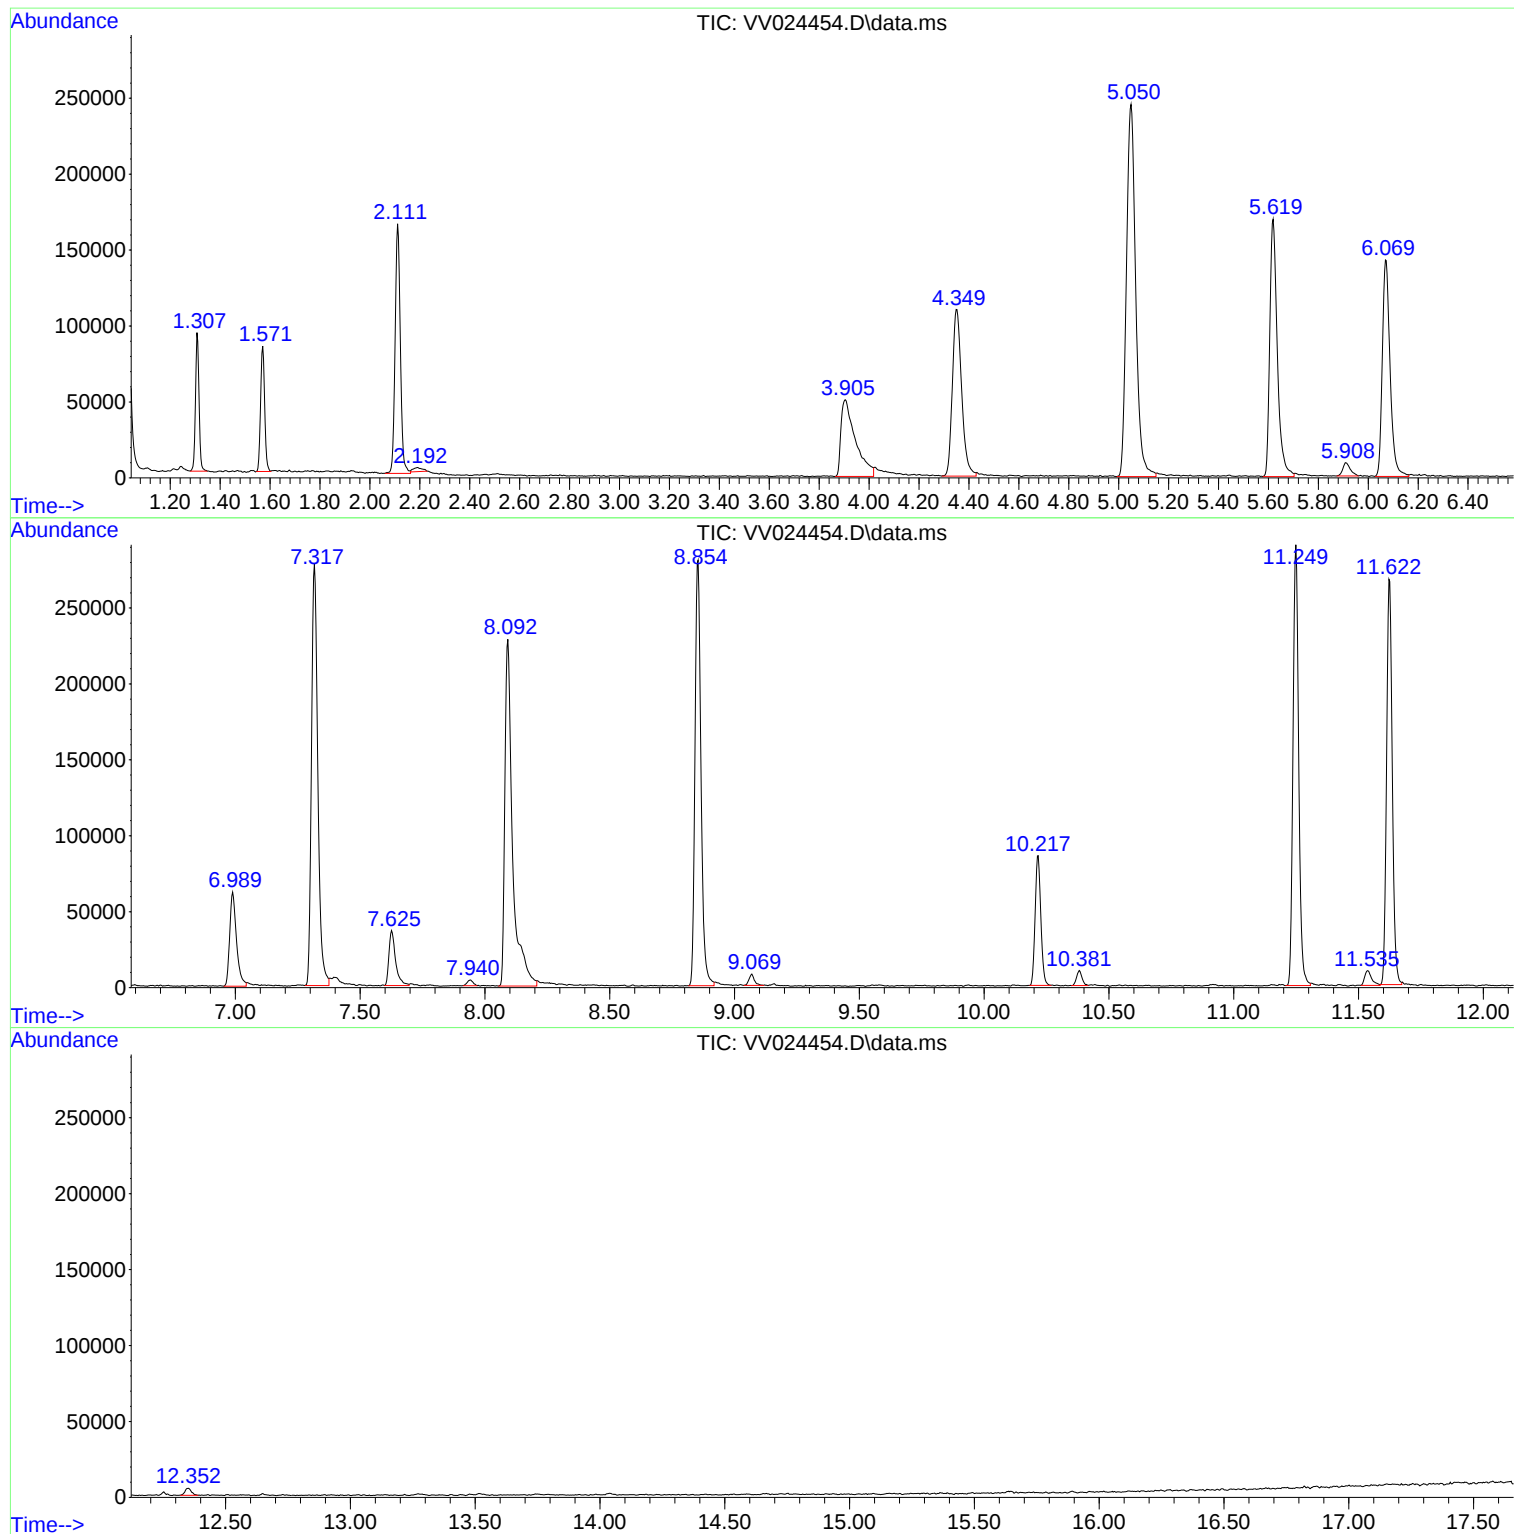

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024454.D
Acq On : 27 Jan 2022 16:13
Operator : SY/MD
Sample : N1275-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024454.D
Acq On : 27 Jan 2022 16:13
Operator : SY/MD
Sample : N1275-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
