

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024461.D
 Acq On : 27 Jan 2022 18:56
 Operator : SY/MD
 Sample : N1317-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	33	rVB	24569	25164	4.25%	0.534%
2	1.217	47	55	61	rVB2	11166	12684	2.14%	0.269%
3	1.307	75	83	93	rVB	89735	96438	16.28%	2.045%
4	1.571	157	165	177	rBV	79112	90781	15.32%	1.925%
5	1.635	179	185	196	rVB2	10404	12831	2.17%	0.272%
6	2.111	323	333	346	rBV	149986	217981	36.79%	4.622%
7	3.899	878	889	917	rBV2	49050	174531	29.46%	3.700%
8	4.349	1014	1029	1055	rBV	107378	272435	45.98%	5.776%
9	5.050	1230	1247	1280	rBV2	232879	592458	100.00%	12.561%
10	5.619	1412	1424	1453	rBV	162177	338909	57.20%	7.186%
11	5.915	1506	1516	1534	rBV8	5964	12291	2.07%	0.261%
12	6.072	1552	1565	1581	rBV2	136953	289220	48.82%	6.132%
13	6.989	1837	1850	1869	rBV	58760	112770	19.03%	2.391%
14	7.317	1941	1952	1970	rBV	254196	454581	76.73%	9.638%
15	7.397	1970	1977	1990	rVB	9518	18061	3.05%	0.383%
16	7.625	2038	2048	2072	rBV3	33557	65638	11.08%	1.392%
17	8.092	2182	2193	2229	rBV	234810	484118	81.71%	10.264%
18	8.355	2264	2275	2288	rVB7	5044	9630	1.63%	0.204%
19	8.854	2417	2430	2455	rBV	272215	455572	76.90%	9.659%
20	10.217	2843	2854	2874	rBV	89557	143713	24.26%	3.047%
21	11.249	3164	3175	3194	rBV	286101	441439	74.51%	9.360%
22	11.622	3280	3291	3309	rBV	243522	395232	66.71%	8.380%




Sum of corrected areas: 4716477

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024461.D
Acq On : 27 Jan 2022 18:56
Operator : SY/MD
Sample : N1317-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

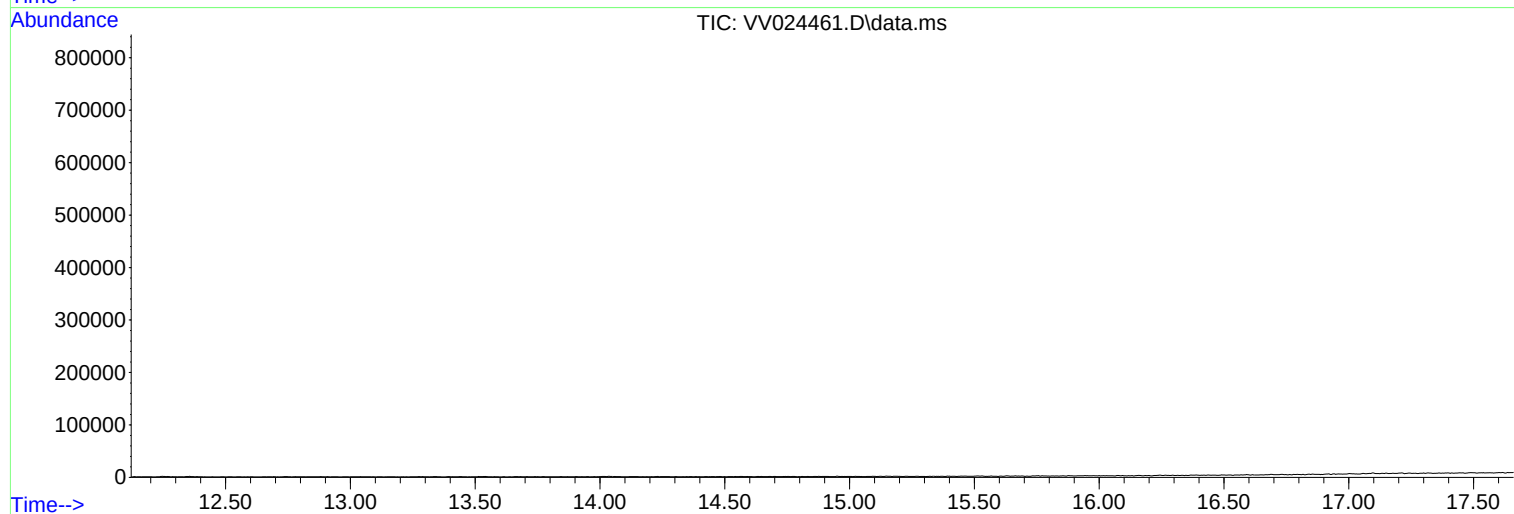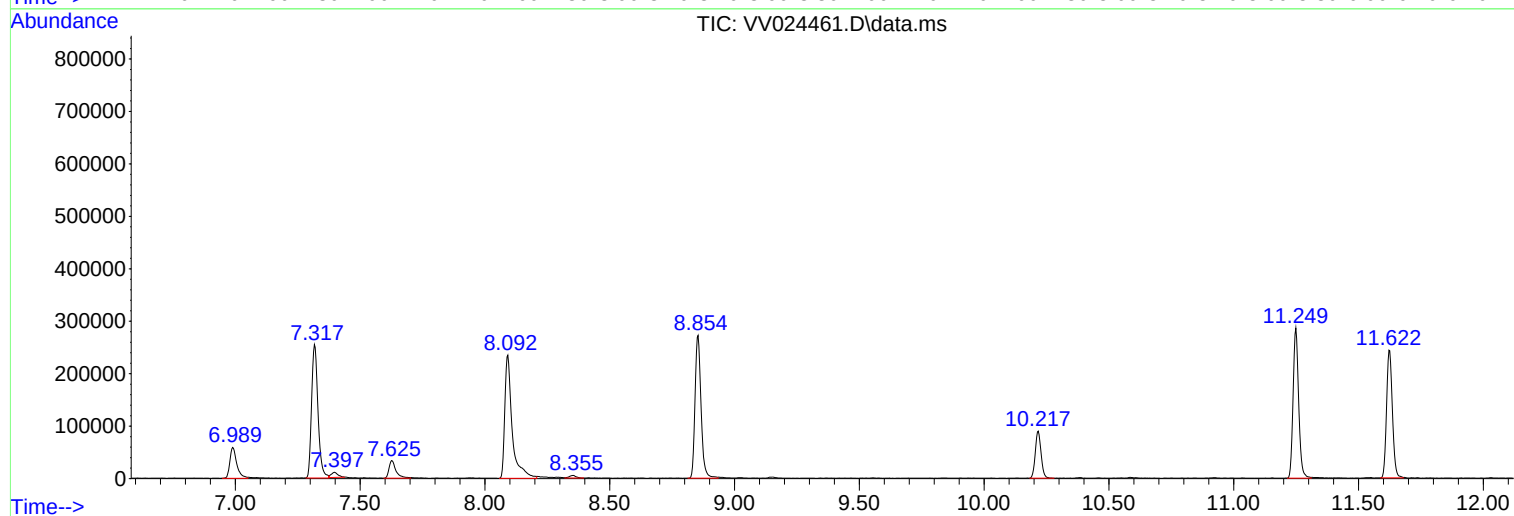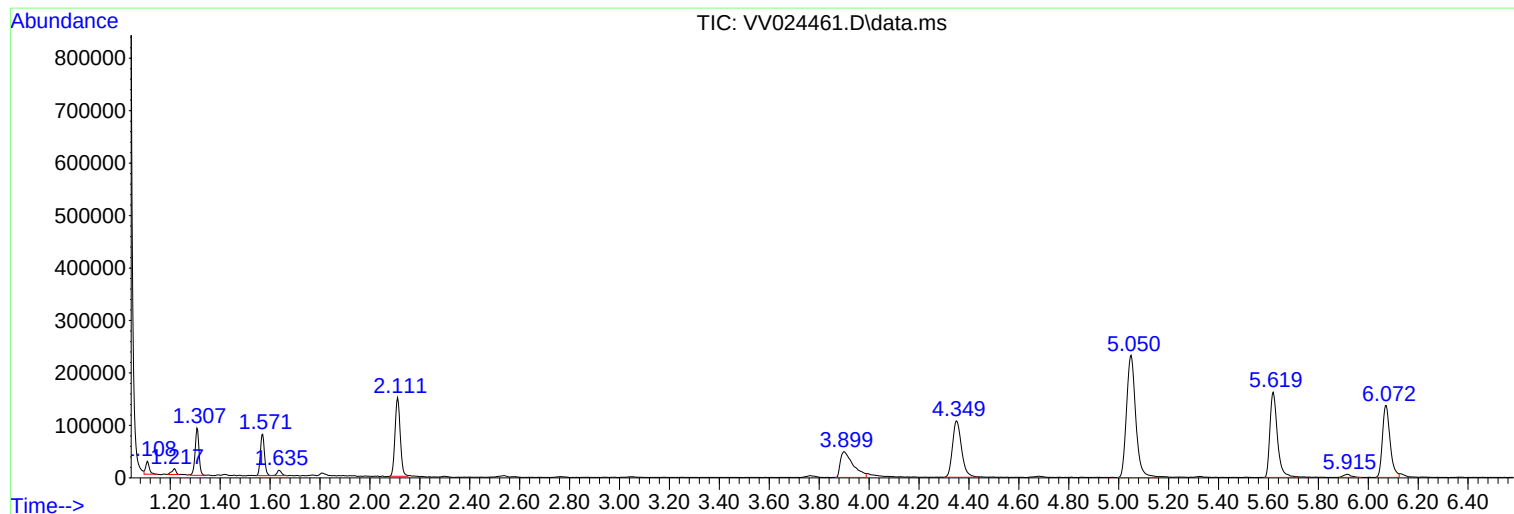

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024461.D
Acq On : 27 Jan 2022 18:56
Operator : SY/MD
Sample : N1317-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024461.D
Acq On : 27 Jan 2022 18:56
Operator : SY/MD
Sample : N1317-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc