

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024462.D
 Acq On : 27 Jan 2022 19:19
 Operator : SY/MD
 Sample : N1317-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rVB	83707	83587	13.64%	1.769%
2	1.417	111	117	127	rVB	13688	15598	2.55%	0.330%
3	1.568	156	164	179	rBV	83847	94942	15.49%	2.009%
4	2.111	322	333	350	rBV	156056	227790	37.17%	4.821%
5	3.909	882	892	922	rBV	37369	152693	24.92%	3.232%
6	4.352	1015	1030	1054	rVB	110228	273048	44.56%	5.779%
7	5.050	1230	1247	1278	rBV2	240842	612799	100.00%	12.970%
8	5.619	1413	1424	1450	rBV	158809	332872	54.32%	7.045%
9	5.915	1504	1516	1527	rBV8	6097	12934	2.11%	0.274%
10	6.069	1552	1564	1594	rBV	140466	295363	48.20%	6.251%
11	6.989	1839	1850	1873	rBV2	58941	113824	18.57%	2.409%
12	7.317	1936	1952	1971	rBV	266719	472825	77.16%	10.007%
13	7.400	1971	1978	1989	rVB3	5944	11330	1.85%	0.240%
14	7.625	2037	2048	2071	rBV	34362	67121	10.95%	1.421%
15	8.092	2183	2193	2230	rBV	222910	517476	84.44%	10.953%
16	8.854	2418	2430	2452	rBV	263015	446353	72.84%	9.447%
17	10.217	2842	2854	2874	rBV2	92517	150284	24.52%	3.181%
18	11.249	3160	3175	3198	rBV	280374	432761	70.62%	9.159%
19	11.622	3279	3291	3307	rBV	257251	411129	67.09%	8.702%




Sum of corrected areas: 4724729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024462.D
Acq On : 27 Jan 2022 19:19
Operator : SY/MD
Sample : N1317-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

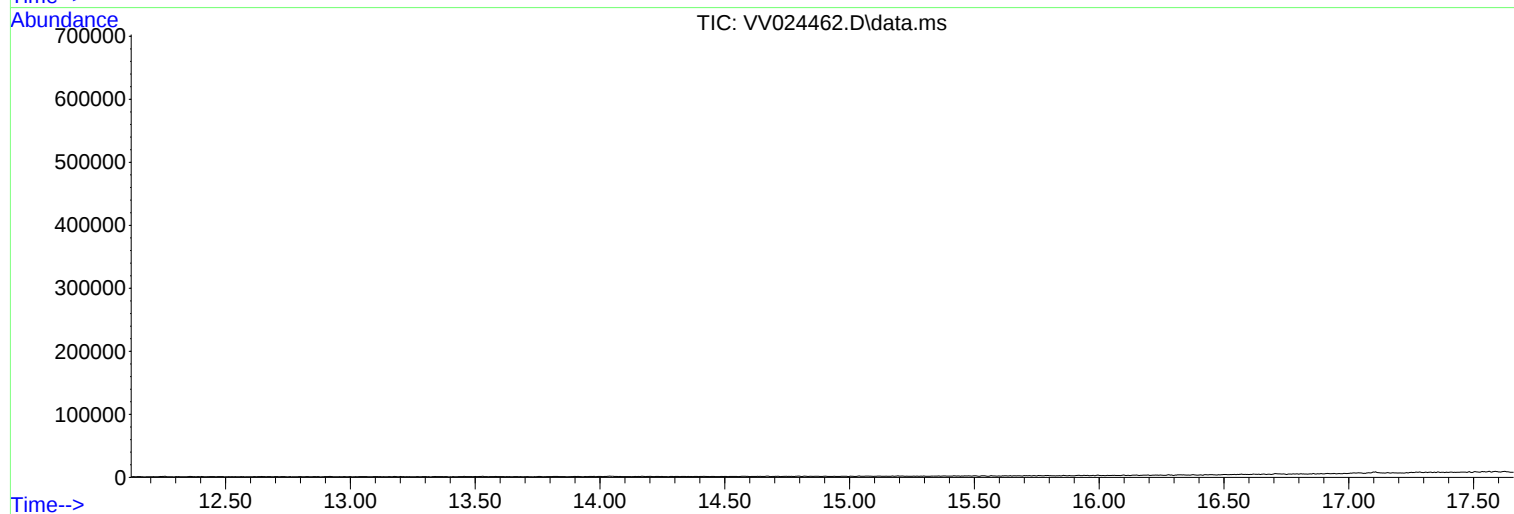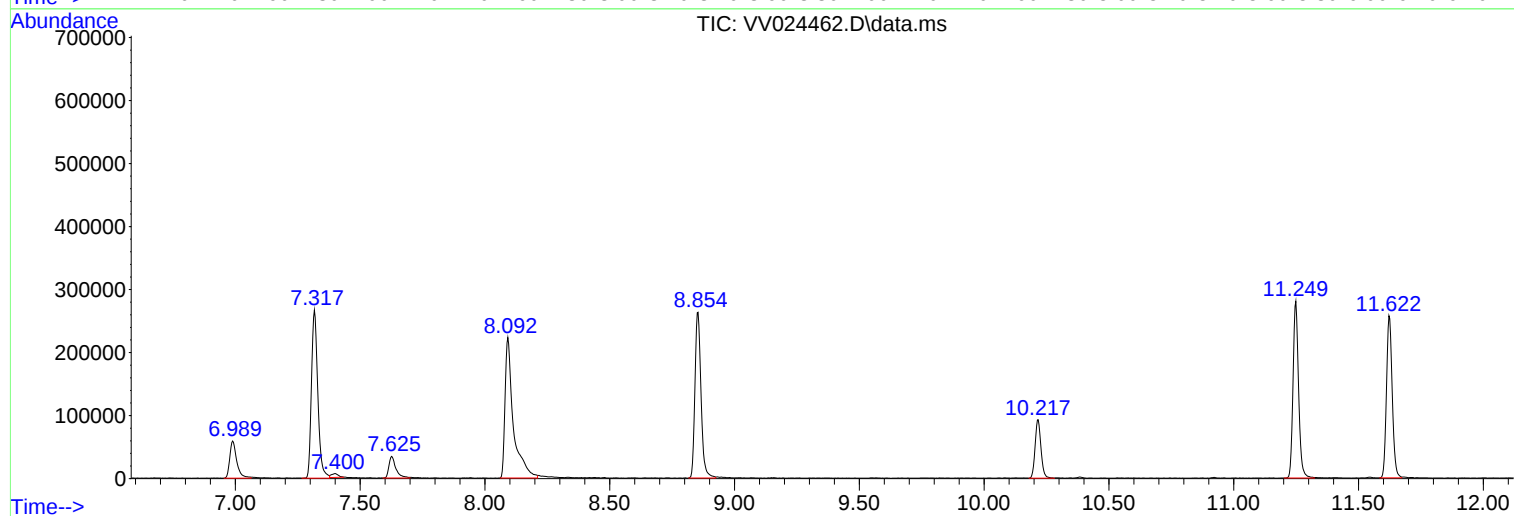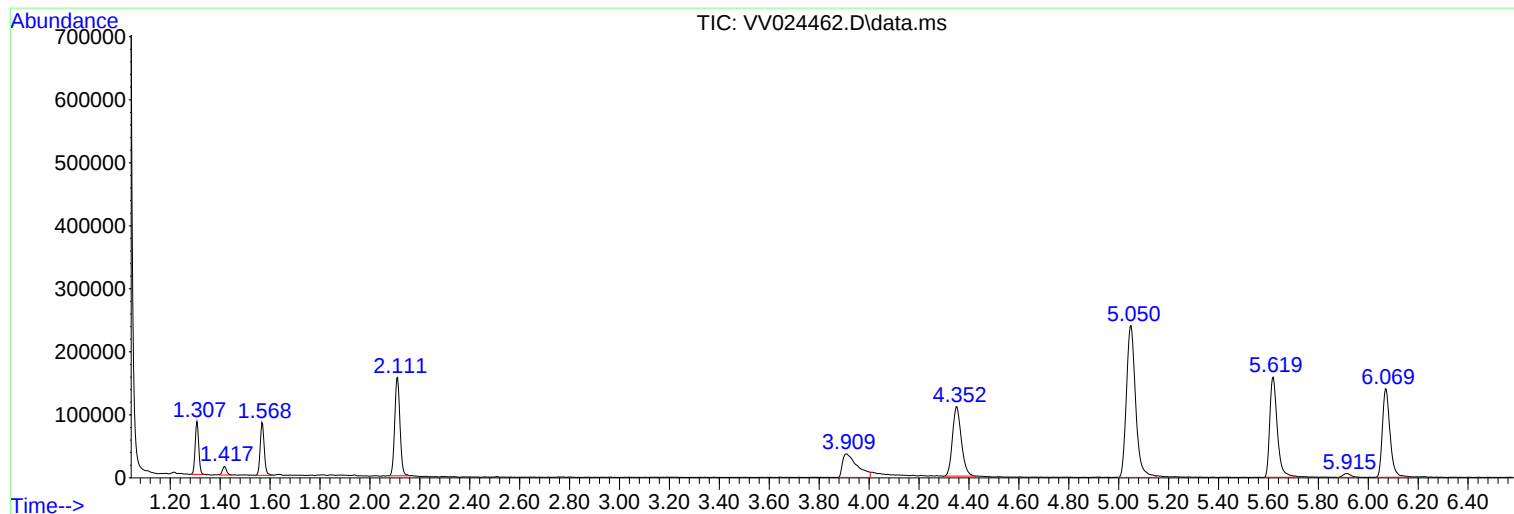

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024462.D
Acq On : 27 Jan 2022 19:19
Operator : SY/MD
Sample : N1317-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024462.D
Acq On : 27 Jan 2022 19:19
Operator : SY/MD
Sample : N1317-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc