

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024463.D
 Acq On : 27 Jan 2022 19:42
 Operator : SY/MD
 Sample : N1317-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	18	21	41	rVB4	10048	13123	2.11%	0.272%
2	1.307	76	83	93	rVB	91219	89511	14.39%	1.853%
3	1.568	156	164	174	rBV	81360	93235	14.99%	1.930%
4	1.635	179	185	196	rVB2	8683	11983	1.93%	0.248%
5	1.809	232	239	247	rVB3	5439	6913	1.11%	0.143%
6	2.108	320	332	348	rVB	159031	230226	37.02%	4.765%
7	3.915	883	894	926	rBV2	31554	143839	23.13%	2.977%
8	4.349	1014	1029	1055	rVB2	111570	278828	44.83%	5.771%
9	5.047	1230	1246	1278	rBV2	245559	621948	100.00%	12.873%
10	5.619	1412	1424	1449	rBV	164718	341770	54.95%	7.074%
11	5.915	1504	1516	1531	rVB5	5833	13652	2.20%	0.283%
12	6.069	1551	1564	1592	rBV	140530	303260	48.76%	6.277%
13	6.989	1841	1850	1874	rBV2	59871	116333	18.70%	2.408%
14	7.317	1941	1952	1971	rBV	270935	481607	77.44%	9.968%
15	7.400	1973	1978	1991	rVB4	5989	10082	1.62%	0.209%
16	7.625	2038	2048	2067	rBV	35130	67016	10.78%	1.387%
17	8.091	2183	2193	2236	rBV	218538	526236	84.61%	10.892%
18	8.853	2416	2430	2450	rBV	273695	457999	73.64%	9.480%
19	10.217	2843	2854	2869	rBV	92376	152044	24.45%	3.147%
20	11.249	3164	3175	3200	rBV	283190	445238	71.59%	9.216%
21	11.625	3280	3292	3310	rBV	263768	426498	68.57%	8.828%




Sum of corrected areas: 4831341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024463.D
Acq On : 27 Jan 2022 19:42
Operator : SY/MD
Sample : N1317-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

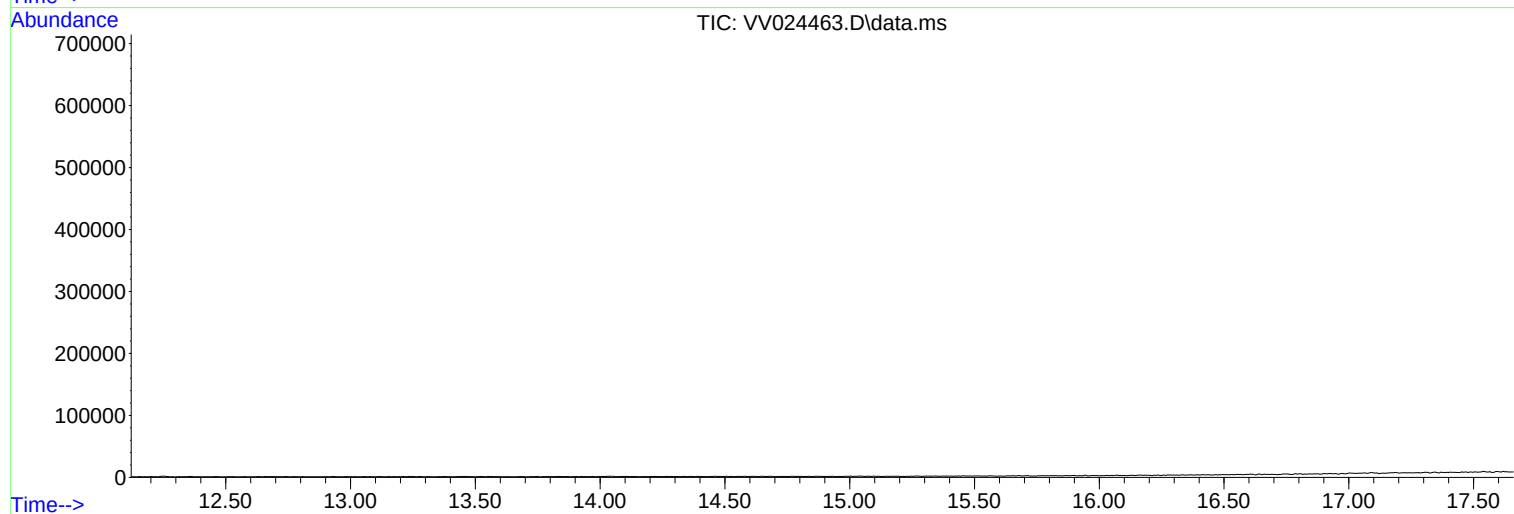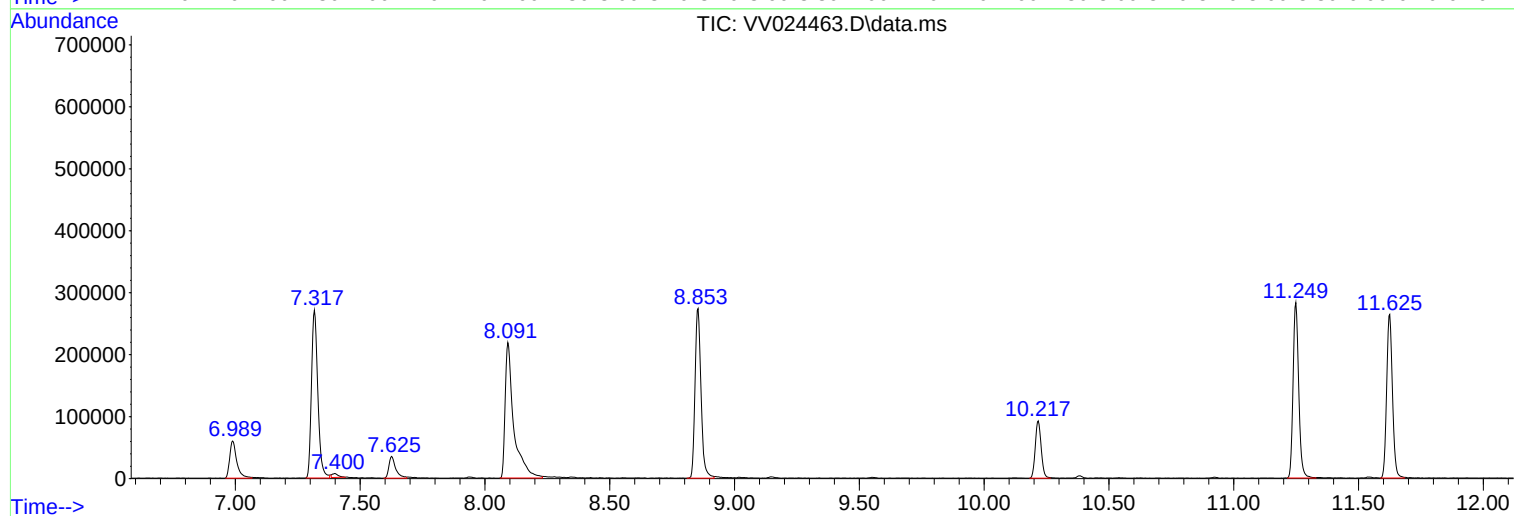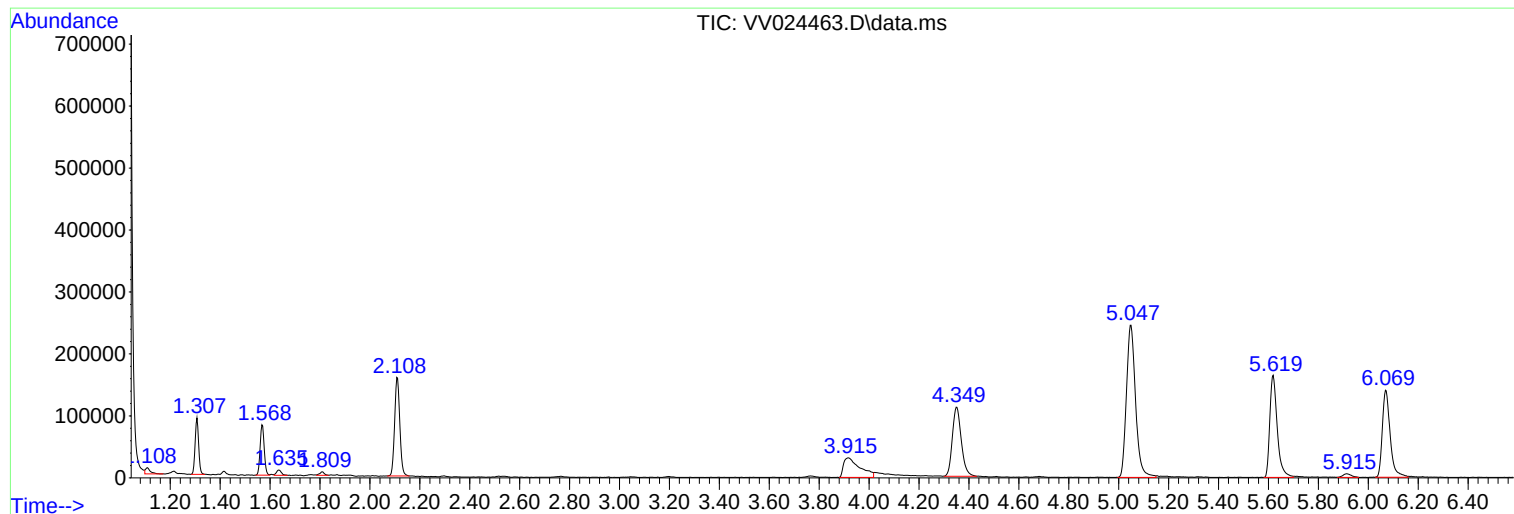

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024463.D
Acq On : 27 Jan 2022 19:42
Operator : SY/MD
Sample : N1317-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024463.D
Acq On : 27 Jan 2022 19:42
Operator : SY/MD
Sample : N1317-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc