

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024467.D
 Acq On : 27 Jan 2022 21:38
 Operator : SY/MD
 Sample : N1318-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P031-TW001-A-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	86192	85870	11.22%	1.535%
2	1.571	157	165	178	rVB	81746	92990	12.15%	1.662%
3	2.111	322	333	353	rVB	155945	229154	29.95%	4.097%
4	3.915	878	894	925	rBV3	79248	266340	34.80%	4.762%
5	4.349	1013	1029	1056	rBV2	109153	283038	36.99%	5.060%
6	4.609	1096	1110	1125	rBV6	6817	16136	2.11%	0.288%
7	5.050	1228	1247	1272	rBV2	243221	613355	80.15%	10.965%
8	5.619	1412	1424	1453	rBV	161517	332408	43.44%	5.943%
9	5.915	1501	1516	1543	rBV	379329	765235	100.00%	13.681%
10	6.069	1551	1564	1592	rBV	141202	296211	38.71%	5.296%
11	6.989	1839	1850	1871	rBV	60271	117875	15.40%	2.107%
12	7.317	1940	1952	1972	rBV	267821	477137	62.35%	8.530%
13	7.625	2039	2048	2065	rBV	34807	65380	8.54%	1.169%
14	8.092	2183	2193	2234	rBV	208633	505409	66.05%	9.035%
15	8.854	2419	2430	2448	rBV	262183	442338	57.80%	7.908%
16	10.217	2842	2854	2868	rBV	90742	146370	19.13%	2.617%
17	11.249	3164	3175	3195	rBV	268927	429266	56.10%	7.674%
18	11.622	3277	3291	3310	rBV	264666	421306	55.06%	7.532%
19	13.506	3868	3877	3887	rBV3	5330	7784	1.02%	0.139%




Sum of corrected areas: 5593602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024467.D
Acq On : 27 Jan 2022 21:38
Operator : SY/MD
Sample : N1318-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-A-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

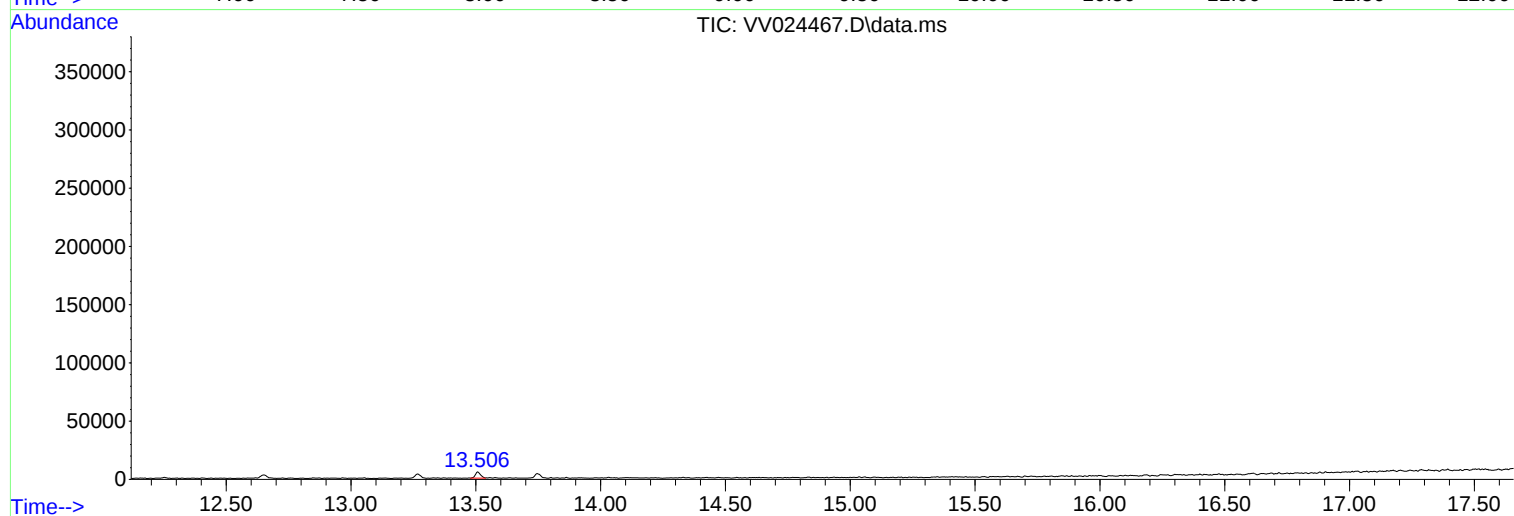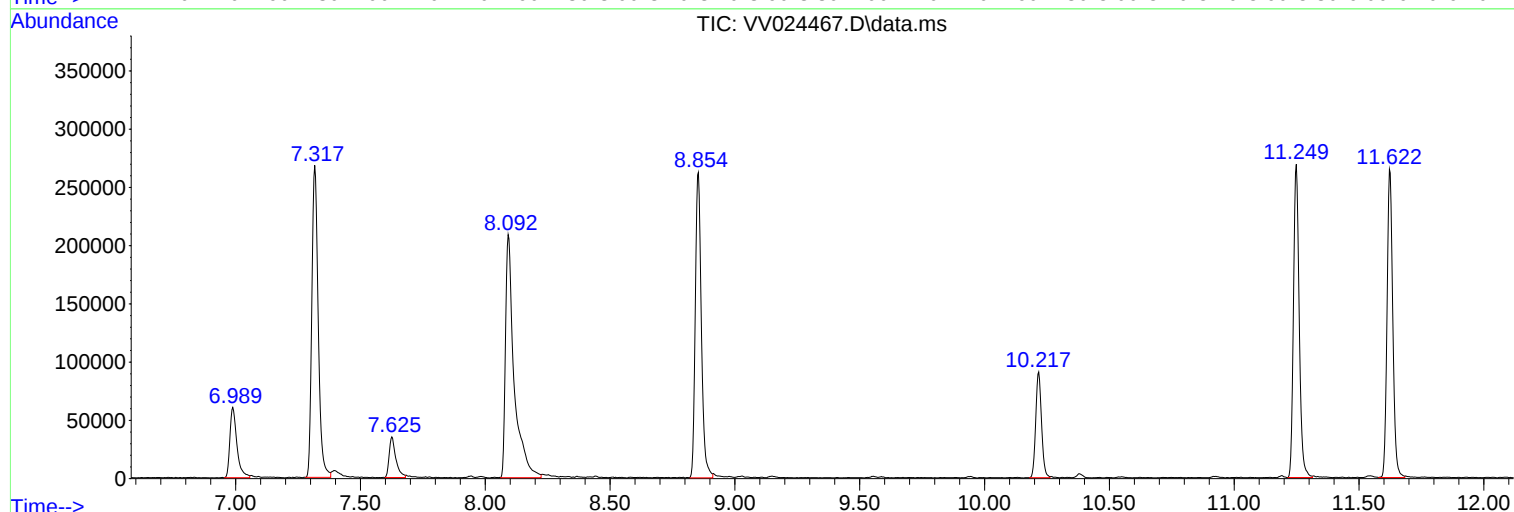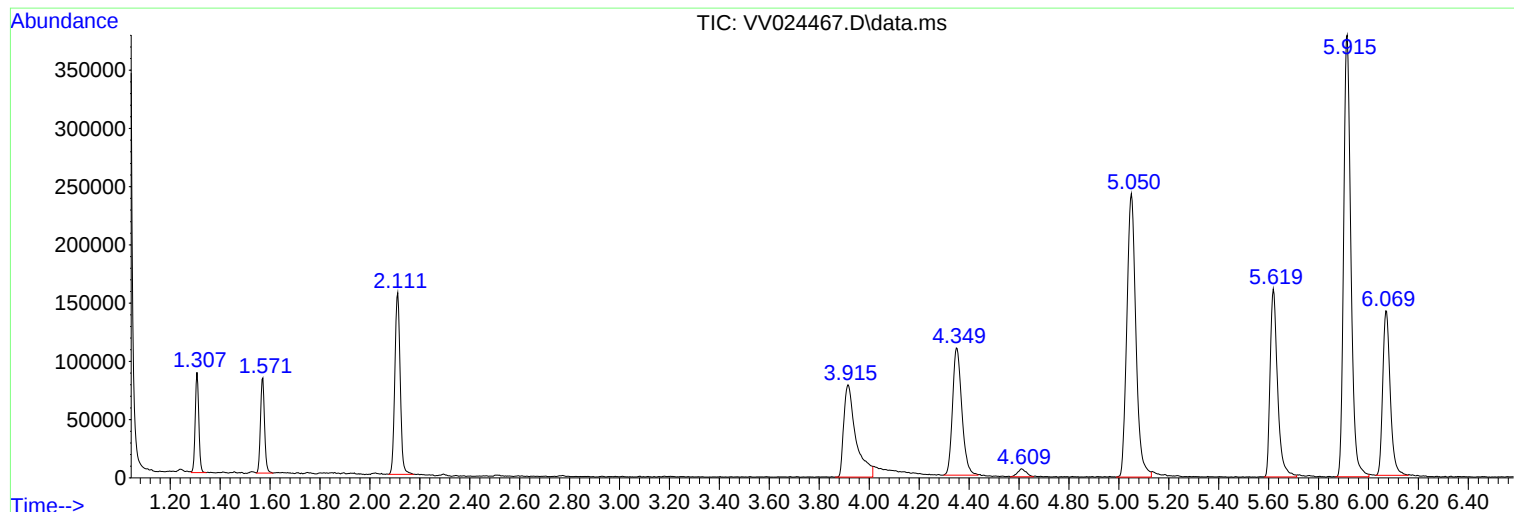

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024467.D
Acq On : 27 Jan 2022 21:38
Operator : SY/MD
Sample : N1318-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-A-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024467.D
Acq On : 27 Jan 2022 21:38
Operator : SY/MD
Sample : N1318-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-A-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------