

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024468.D
 Acq On : 27 Jan 2022 22:02
 Operator : SY/MD
 Sample : N1318-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P031-TW001-A-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	72	rVB	12099	13074	1.74%	0.237%
2	1.307	76	83	97	rVB	81834	83344	11.10%	1.512%
3	1.568	157	164	177	rBV	80452	91736	12.21%	1.665%
4	2.111	322	333	345	rBV	151676	222597	29.64%	4.039%
5	3.915	882	894	931	rBV3	77443	268830	35.79%	4.878%
6	4.352	1013	1030	1055	rBV	106268	273253	36.38%	4.958%
7	4.613	1097	1111	1128	rVB3	5773	15323	2.04%	0.278%
8	5.050	1230	1247	1292	rBV2	235783	603038	80.29%	10.942%
9	5.619	1413	1424	1448	rBV	159770	332459	44.26%	6.032%
10	5.915	1502	1516	1543	rBV	372084	751071	100.00%	13.628%
11	6.069	1552	1564	1587	rBV2	135352	285137	37.96%	5.174%
12	6.989	1838	1850	1874	rBV	58900	113806	15.15%	2.065%
13	7.317	1940	1952	1970	rBV	260193	459669	61.20%	8.341%
14	7.625	2039	2048	2066	rBV2	34935	64154	8.54%	1.164%
15	8.092	2183	2193	2232	rBV	207554	493464	65.70%	8.954%
16	8.854	2418	2430	2451	rBV	268150	446752	59.48%	8.106%
17	10.217	2842	2854	2873	rBV	89744	140927	18.76%	2.557%
18	10.384	2894	2906	2917	rVB2	8437	13668	1.82%	0.248%
19	11.249	3163	3175	3199	rBV	274411	432503	57.58%	7.848%
20	11.622	3280	3291	3313	rBV	250054	406459	54.12%	7.375%




Sum of corrected areas: 5511264

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024468.D
Acq On : 27 Jan 2022 22:02
Operator : SY/MD
Sample : N1318-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-A-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

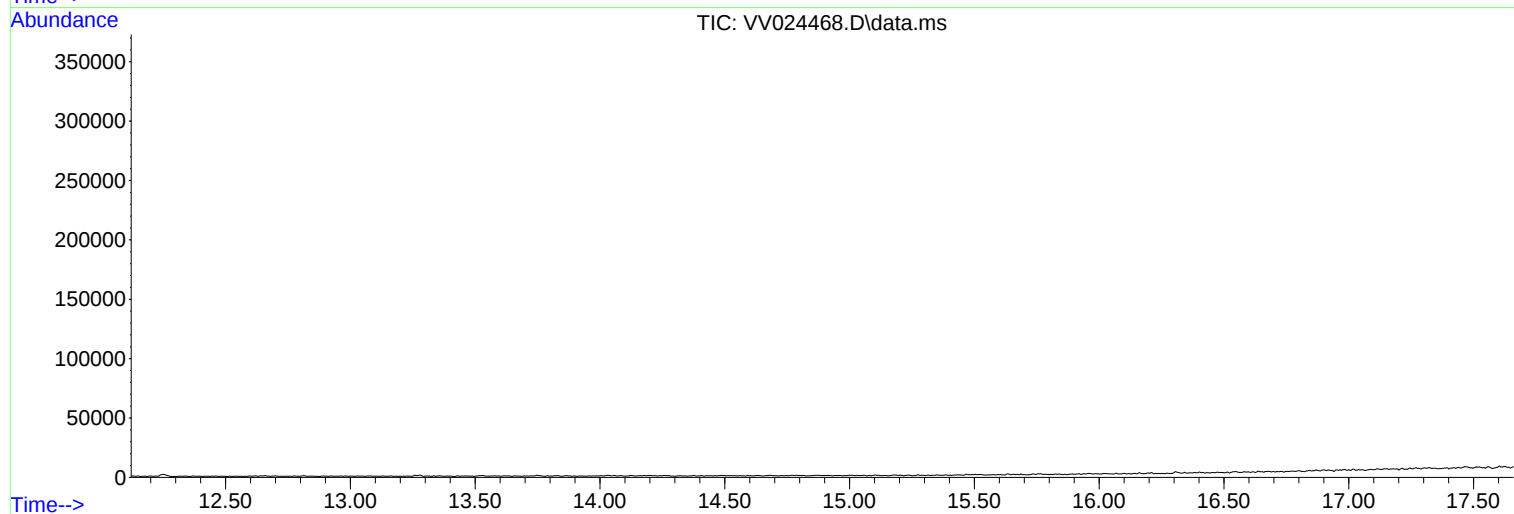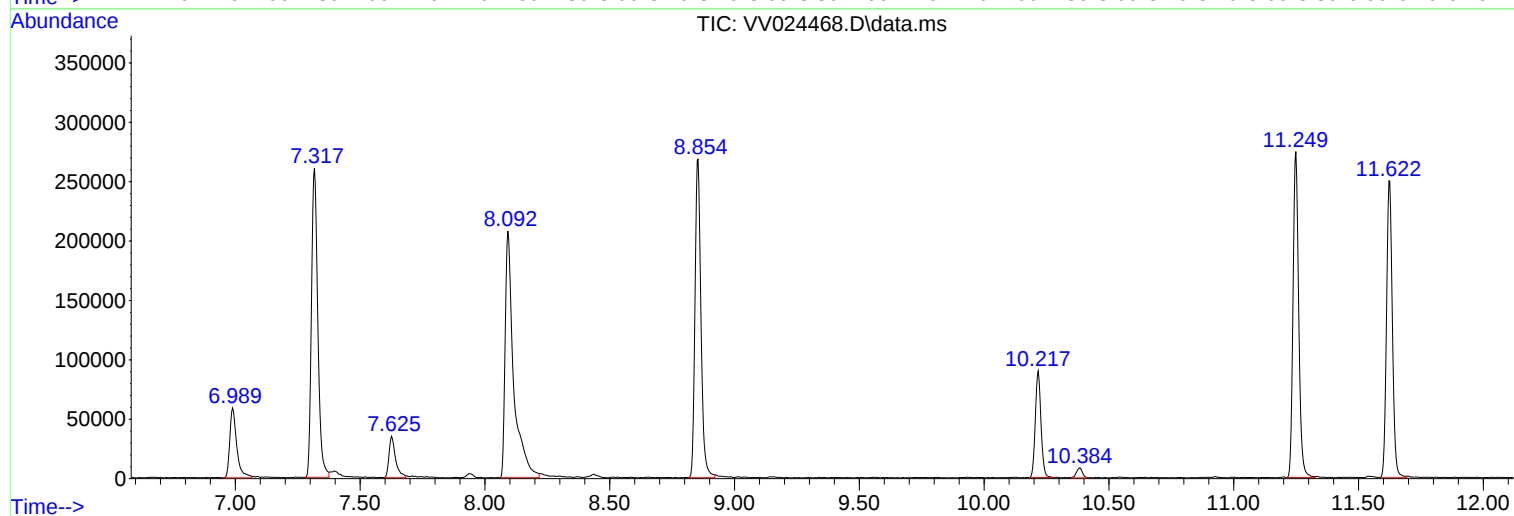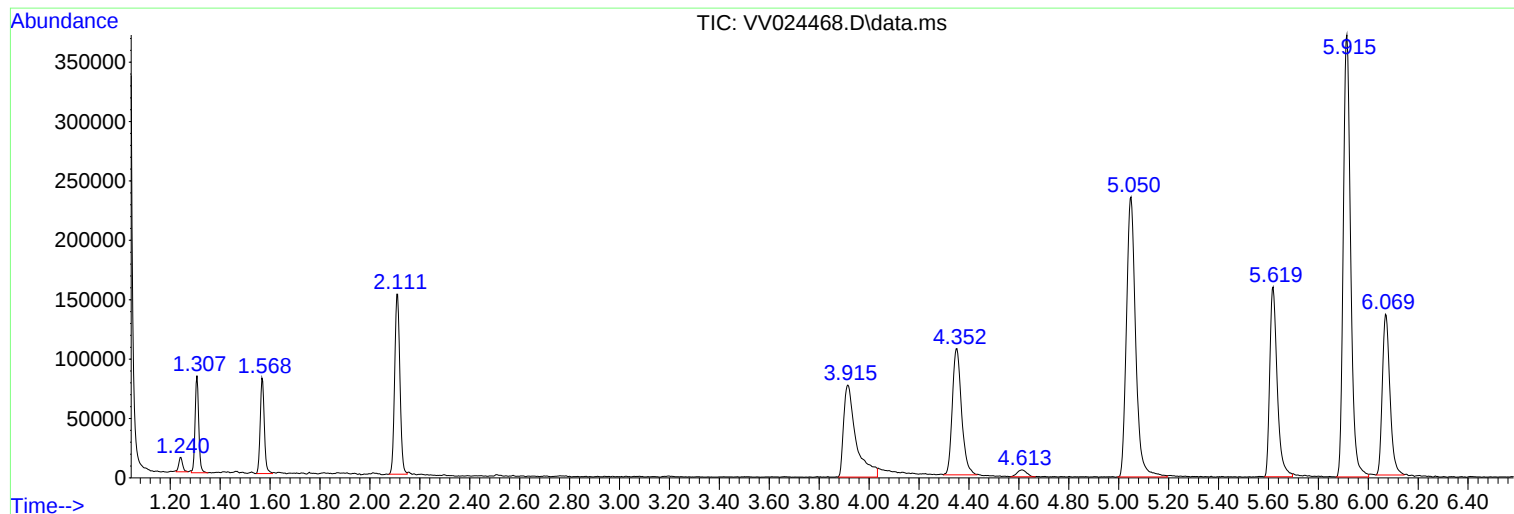

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024468.D
Acq On : 27 Jan 2022 22:02
Operator : SY/MD
Sample : N1318-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-A-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024468.D
Acq On : 27 Jan 2022 22:02
Operator : SY/MD
Sample : N1318-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-A-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc