

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024470.D
 Acq On : 27 Jan 2022 22:48
 Operator : SY/MD
 Sample : N1318-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P031-TW001-C-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rVB	79267	79295	13.88%	1.766%
2	1.568	157	164	174	rBV	75509	85949	15.04%	1.914%
3	2.111	322	333	350	rBV	144853	212631	37.21%	4.736%
4	3.905	880	891	934	rBV	45432	188799	33.04%	4.205%
5	4.349	1013	1029	1056	rBV2	102384	265070	46.39%	5.904%
6	5.050	1230	1247	1274	rBV2	224857	571434	100.00%	12.727%
7	5.619	1411	1424	1449	rBV	159973	328895	57.56%	7.325%
8	5.915	1504	1516	1530	rBV7	5619	12862	2.25%	0.286%
9	6.069	1552	1564	1595	rBV	132638	280789	49.14%	6.254%
10	6.989	1839	1850	1870	rBV	54460	105542	18.47%	2.351%
11	7.317	1940	1952	1970	rBV	245258	434039	75.96%	9.667%
12	7.625	2039	2048	2062	rBV	32790	59182	10.36%	1.318%
13	7.941	2136	2146	2156	rBV5	3328	5917	1.04%	0.132%
14	8.092	2181	2193	2231	rBV	214272	460469	80.58%	10.256%
15	8.854	2419	2430	2453	rBV	266363	443479	77.61%	9.877%
16	10.214	2842	2853	2867	rBV	85415	137080	23.99%	3.053%
17	10.381	2896	2905	2916	rVB3	7965	12614	2.21%	0.281%
18	11.249	3164	3175	3195	rBV	267663	423192	74.06%	9.425%
19	11.625	3277	3292	3317	rBV	234482	382702	66.97%	8.524%




Sum of corrected areas: 4489940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024470.D
Acq On : 27 Jan 2022 22:48
Operator : SY/MD
Sample : N1318-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-C-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

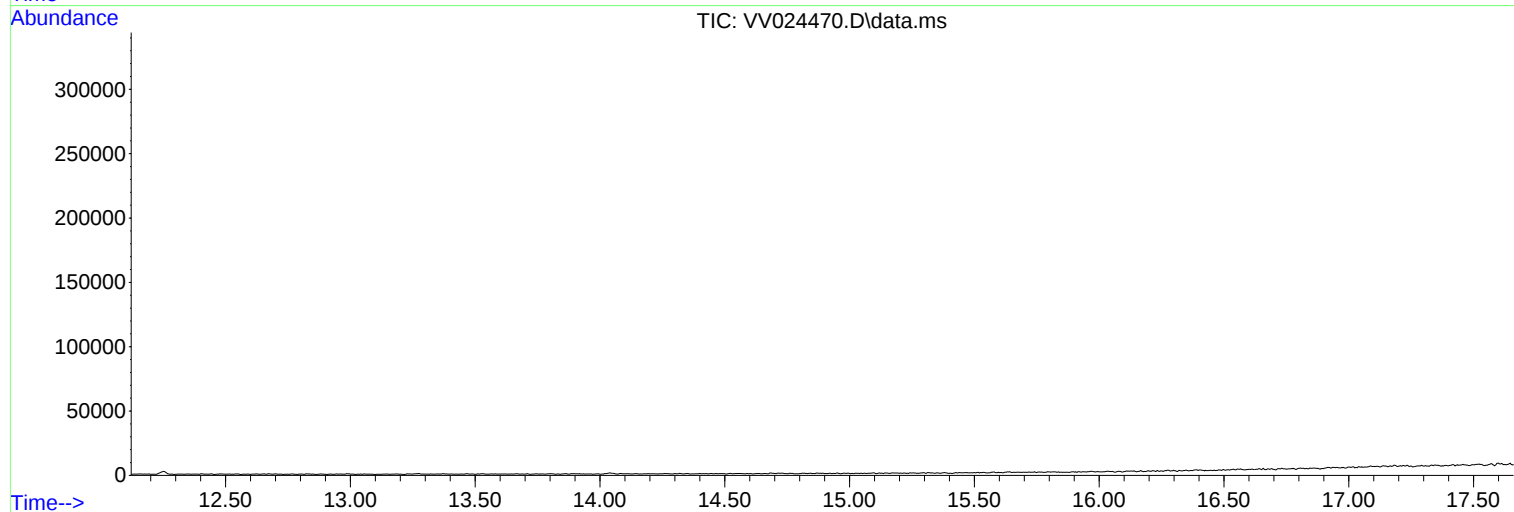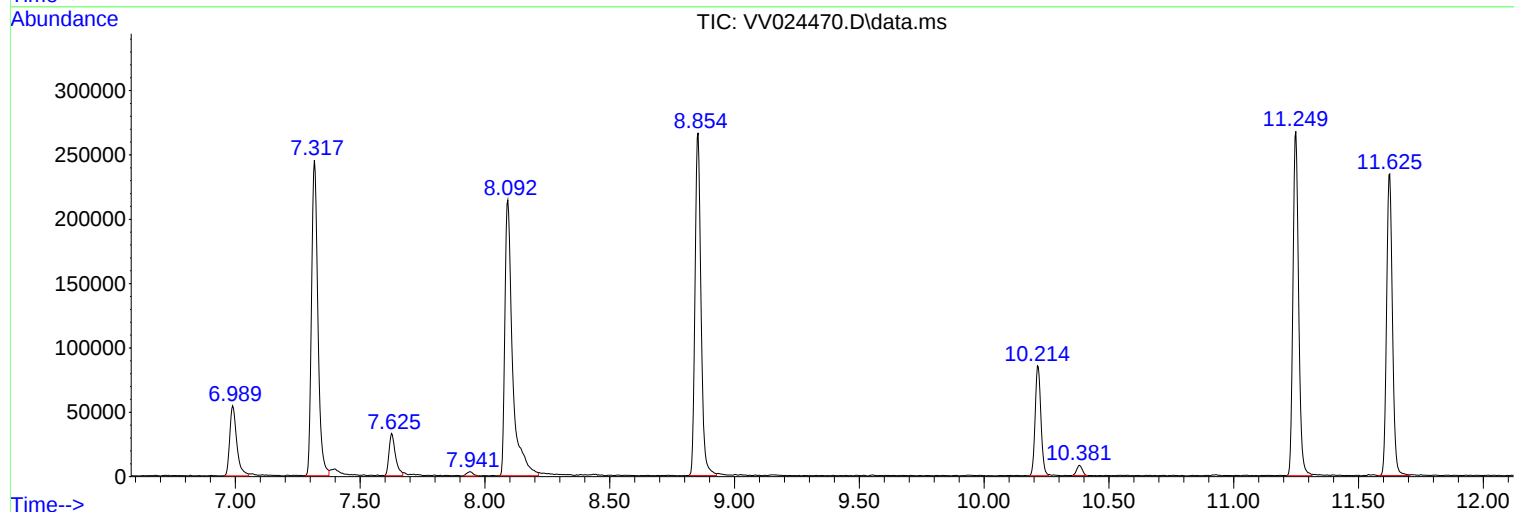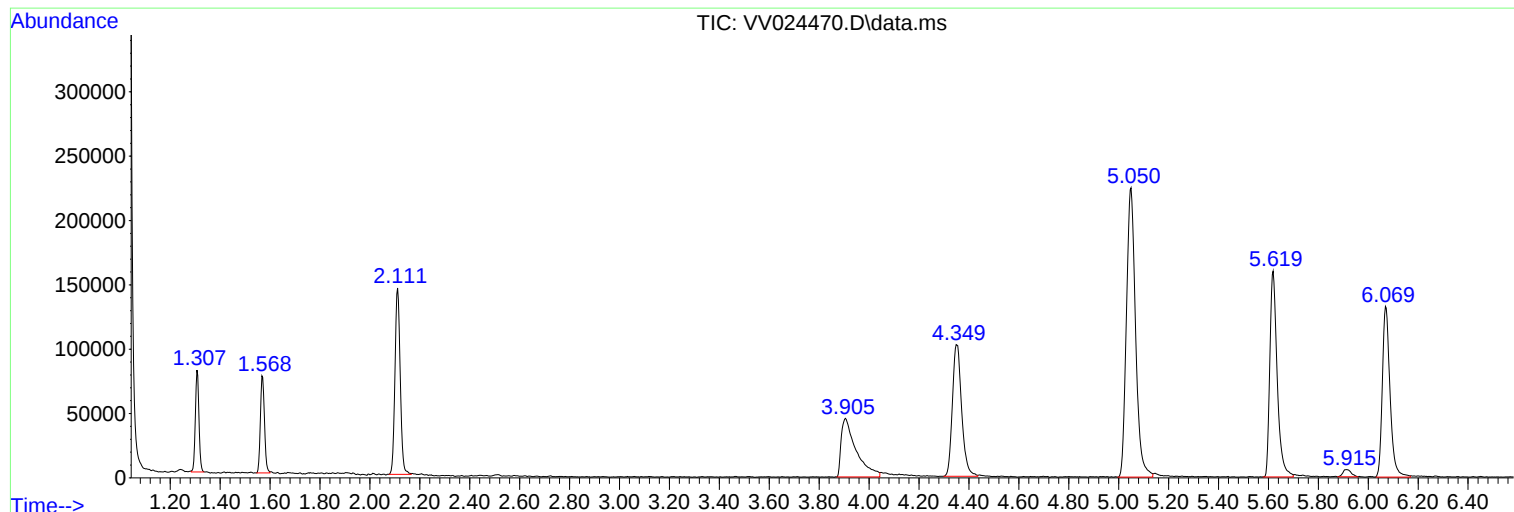

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024470.D
Acq On : 27 Jan 2022 22:48
Operator : SY/MD
Sample : N1318-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-C-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024470.D
Acq On : 27 Jan 2022 22:48
Operator : SY/MD
Sample : N1318-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P031-TW001-C-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------