

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024472.D
 Acq On : 27 Jan 2022 23:35
 Operator : SY/MD
 Sample : N1317-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rVB	87787	87733	14.70%	1.884%
2	1.568	156	164	181	rBV	78900	93079	15.60%	1.999%
3	2.108	322	332	348	rVB	151204	222489	37.28%	4.778%
4	3.921	884	896	925	rBV	28366	128336	21.50%	2.756%
5	4.349	1014	1029	1056	rBV	109464	272817	45.71%	5.859%
6	5.050	1231	1247	1278	rBV2	237448	596805	100.00%	12.817%
7	5.619	1411	1424	1449	rBV	156449	328867	55.10%	7.063%
8	5.915	1505	1516	1526	rBV8	6337	13428	2.25%	0.288%
9	6.069	1549	1564	1592	rBV2	139927	295456	49.51%	6.345%
10	6.989	1840	1850	1874	rBV	57006	111055	18.61%	2.385%
11	7.317	1940	1952	1970	rBV	257602	454694	76.19%	9.765%
12	7.625	2037	2048	2070	rBV	32805	63110	10.57%	1.355%
13	7.940	2131	2146	2156	rBV2	7661	14141	2.37%	0.304%
14	8.092	2183	2193	2235	rBV	198204	500322	83.83%	10.745%
15	8.854	2418	2430	2458	rBV	267941	449826	75.37%	9.660%
16	10.217	2842	2854	2871	rBV	90529	146927	24.62%	3.155%
17	10.381	2892	2905	2919	rVB	20663	34119	5.72%	0.733%
18	11.249	3161	3175	3198	rBV	271133	431309	72.27%	9.263%
19	11.625	3280	3292	3318	rBV	250266	404113	67.71%	8.679%
20	12.252	3478	3487	3496	rBV3	5262	7725	1.29%	0.166%




Sum of corrected areas: 4656351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024472.D
Acq On : 27 Jan 2022 23:35
Operator : SY/MD
Sample : N1317-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

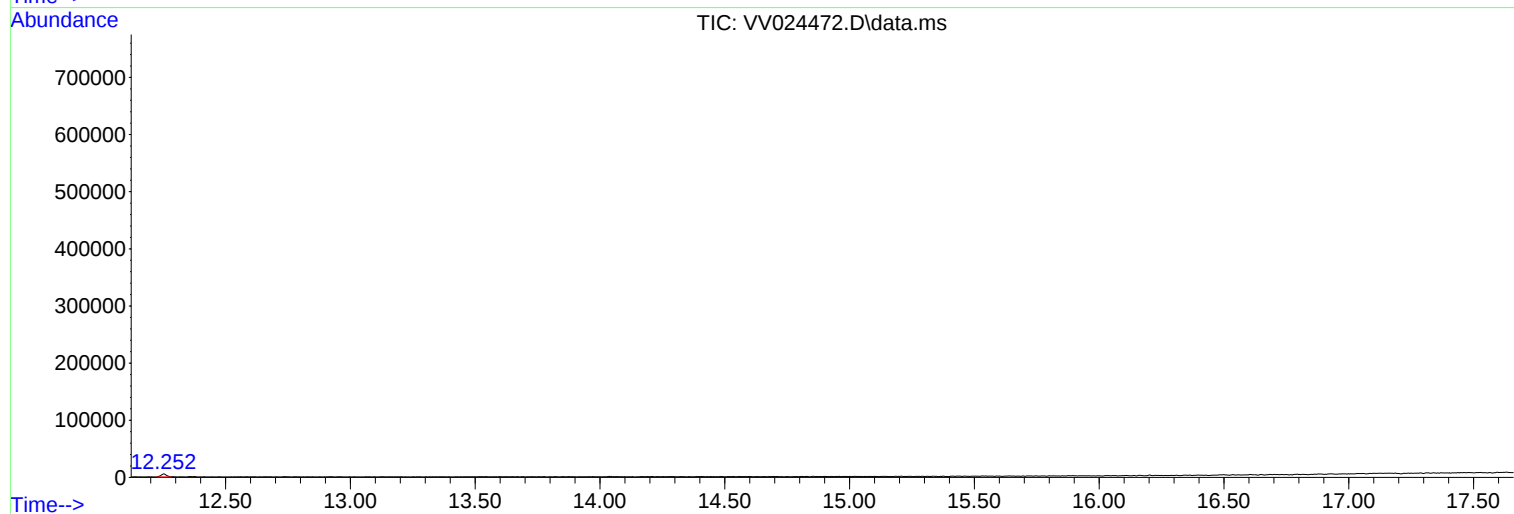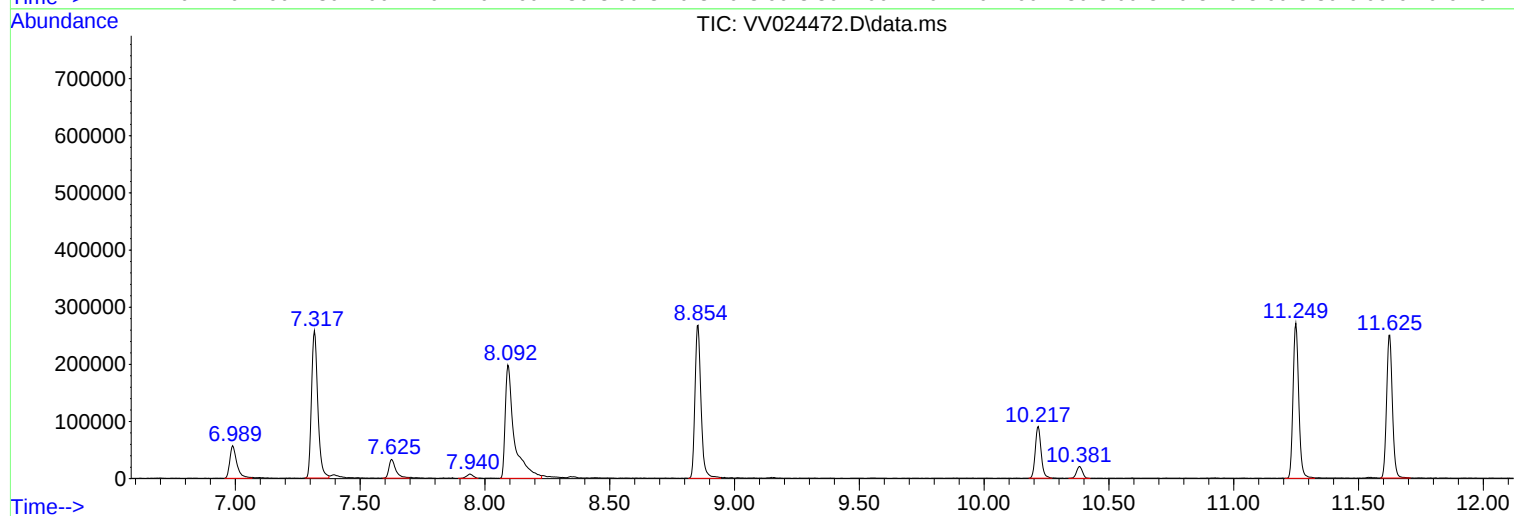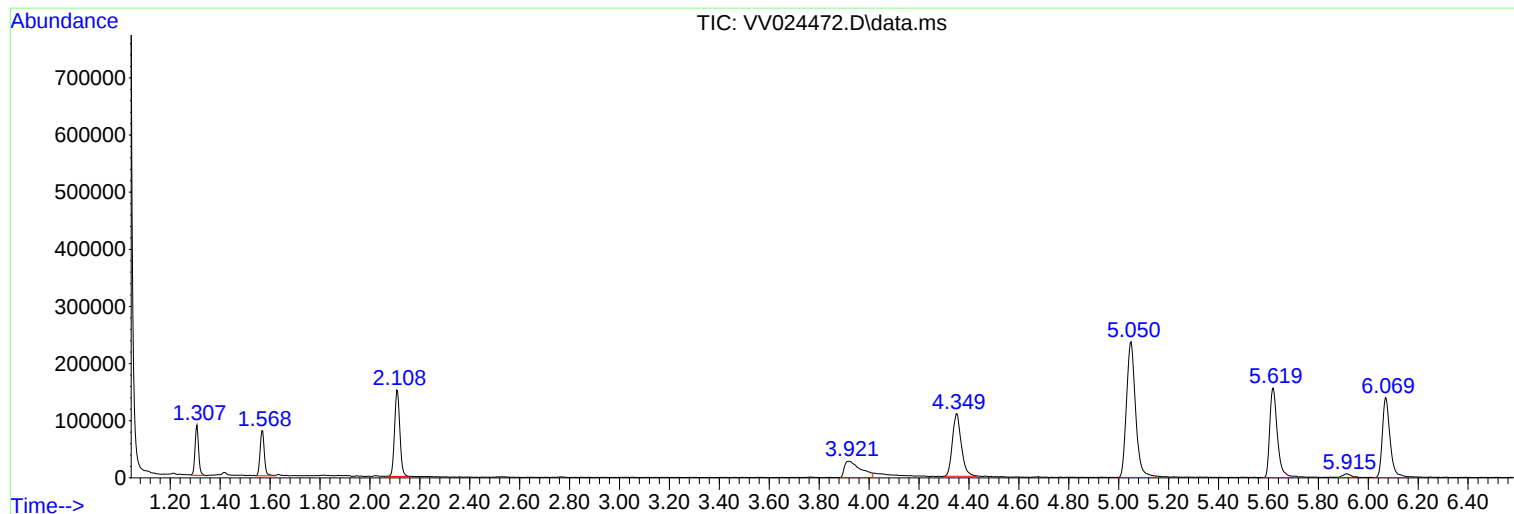

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024472.D
Acq On : 27 Jan 2022 23:35
Operator : SY/MD
Sample : N1317-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
Data File : VV024472.D
Acq On : 27 Jan 2022 23:35
Operator : SY/MD
Sample : N1317-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc