
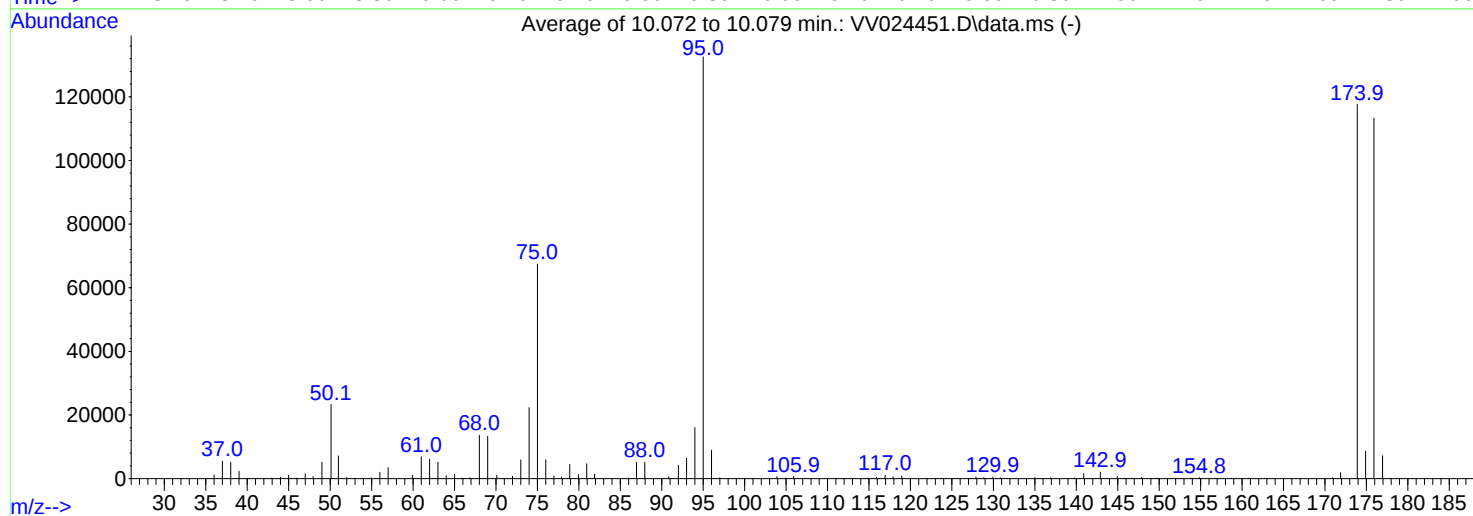


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012722\
 Data File : VV024451.D
 Acq On : 27 Jan 2022 13:57
 Operator : SY/MD
 Sample : BFB264
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB264

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jan 28 03:20:33 2022

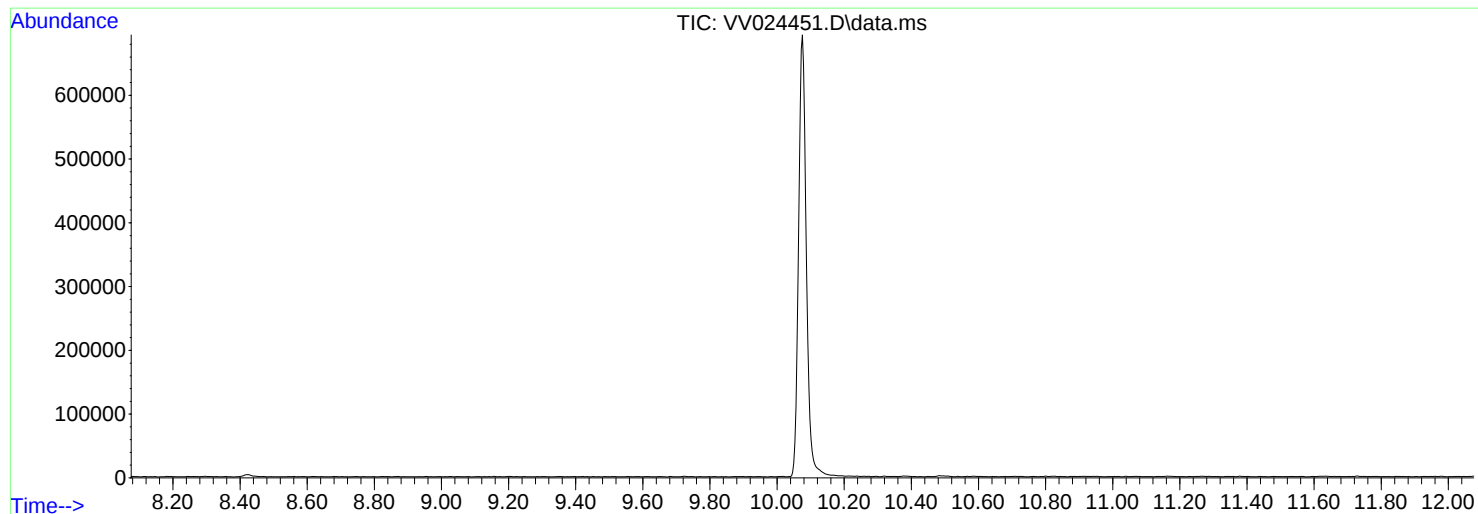

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	23320	PASS
75	95	30	80	50.9	67448	PASS
95	95	100	100	100.0	132576	PASS
96	95	5	9	6.8	8957	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.7	117611	PASS
175	174	5	9	7.3	8634	PASS
176	174	95	105	96.3	113301	PASS
177	176	5	10	6.3	7178	PASS

m/z	Abundance
36.00	1077.0
37.00	5215.0
38.00	4917.0
39.00	2147.0
39.90	225.0
42.90	159.0
44.00	2169.0
45.00	905.0
46.00	216.0
47.00	1402.0
47.90	790.0
49.00	4921.0
50.10	22776.0
51.00	6820.0
52.00	329.0
53.00	157.0
54.90	315.0
56.00	1882.0
57.00	3373.0
58.00	141.0
60.00	1036.0
61.00	6358.0
62.00	5678.0
63.00	4687.0
64.00	871.0
65.00	1465.0
65.90	148.0
66.80	312.0
68.00	12633.0
69.00	12704.0
70.10	1084.0
72.00	807.0
73.00	5790.0
74.00	21728.0
75.00	64552.0
76.00	5643.0
77.00	830.0
77.90	503.0
78.90	4227.0
79.90	1325.0
81.00	4396.0
81.90	1347.0
85.90	251.0
87.00	4857.0
88.00	4986.0
90.80	609.0
92.00	4075.0
93.00	6167.0
94.00	15488.0
95.00	126496.0
96.00	8309.0
97.00	272.0
103.90	593.0
105.00	176.0
105.90	654.0
106.90	110.0
111.00	141.0
113.00	116.0
114.90	138.0
115.90	477.0
116.90	975.0
117.90	531.0
119.00	868.0
123.80	122.0
127.10	101.0
127.90	519.0
128.90	337.0
129.90	505.0
130.80	233.0
135.00	295.0
136.90	293.0
139.80	177.0
140.90	1473.0
141.90	232.0
142.90	1935.0
144.00	168.0
144.90	588.0
146.00	178.0
147.90	400.0
149.70	217.0
151.90	114.0
152.90	128.0
153.80	107.0
154.90	330.0
156.80	156.0
157.10	155.0
158.70	152.0
160.90	179.0
170.90	250.0
171.90	1849.0
173.90	115408.0
174.90	8300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

175.90	110872.0
176.90	7097.0
177.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
39.90	214.0
44.00	1664.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
36.00	1203.0
37.00	5592.0
38.00	5272.0
39.00	2457.0
40.20	238.0
41.30	112.0
42.90	227.0
44.00	2109.0
45.00	1183.0
46.00	231.0
47.00	1544.0
48.00	566.0
49.00	5131.0
50.10	23176.0
51.00	7174.0
52.00	355.0
53.00	244.0
53.90	129.0
55.00	354.0
56.00	2040.0
57.00	3436.0
58.00	189.0
59.90	1180.0
61.00	7051.0
62.00	6431.0
63.00	5356.0
64.00	932.0
65.00	1412.0
65.90	137.0
66.10	146.0
66.90	330.0
68.00	14006.0
69.00	13295.0
70.10	1088.0
72.00	728.0
73.00	5757.0
74.00	22200.0
75.00	67920.0
76.00	6038.0
77.00	773.0
77.90	526.0
78.90	4605.0
80.00	1207.0
80.90	4800.0
81.90	1336.0
82.80	116.0
86.00	223.0
86.90	5239.0
87.90	5126.0
90.90	516.0
92.00	4144.0
93.00	6306.0
94.00	16040.0
95.00	134080.0
96.00	9260.0
97.00	372.0
103.90	674.0
104.90	228.0
105.90	650.0
107.00	170.0
111.00	159.0
111.90	107.0
113.00	126.0
114.80	139.0
115.90	467.0
117.00	1118.0
117.90	566.0
118.90	847.0
123.80	135.0
127.90	513.0
128.80	304.0
130.00	527.0
130.90	232.0
135.00	317.0
136.90	288.0
139.80	140.0
140.90	1557.0
142.90	2023.0
144.00	161.0
145.00	704.0
145.80	225.0
146.80	120.0
147.90	410.0
149.80	168.0
152.00	119.0
153.80	147.0
154.80	339.0
156.30	126.0
156.70	175.0
157.20	107.0
158.80	173.0
160.80	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

171.00	314.0
171.90	1862.0
173.90	115800.0
174.90	8719.0
175.90	112008.0
177.00	7024.0
178.00	174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
36.00	1224.0
37.00	5640.0
38.00	5375.0
39.00	2379.0
39.90	246.0
42.90	213.0
44.00	2099.0
45.00	1124.0
46.00	234.0
47.00	1542.0
47.90	691.0
49.00	5334.0
50.10	24008.0
51.00	7394.0
52.00	380.0
53.00	227.0
53.90	116.0
54.90	330.0
56.00	2093.0
57.00	3685.0
58.00	186.0
60.00	1160.0
61.00	7113.0
62.00	6332.0
63.00	5307.0
64.00	910.0
65.00	1508.0
65.80	145.0
66.90	308.0
68.00	14278.0
69.00	13793.0
70.10	1128.0
72.00	808.0
73.00	6177.0
74.00	23056.0
75.00	69872.0
76.00	6212.0
77.00	878.0
77.90	557.0
78.90	4629.0
79.90	1329.0
81.00	4815.0
81.90	1439.0
86.00	239.0
86.90	5300.0
87.90	5346.0
90.90	577.0
92.00	4346.0
93.00	6670.0
94.00	16552.0
95.00	137152.0
96.00	9301.0
97.00	330.0
103.00	105.0
103.90	650.0
104.90	197.0
105.90	695.0
107.00	134.0
111.10	155.0
112.00	103.0
113.00	123.0
114.80	137.0
115.90	487.0
117.00	1094.0
117.90	576.0
118.90	895.0
123.80	134.0
125.70	108.0
127.00	108.0
127.90	536.0
128.90	362.0
130.00	560.0
130.90	248.0
135.00	331.0
136.90	311.0
139.80	177.0
140.90	1613.0
141.90	176.0
142.90	2048.0
144.00	186.0
145.00	675.0
145.80	194.0
147.90	439.0
149.70	214.0
152.00	118.0
152.90	103.0
153.80	144.0
154.90	351.0
156.80	165.0
158.70	177.0
160.80	205.0
171.00	293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

171.90	2000.0
173.90	121624.0
174.90	8882.0
175.90	117024.0
176.90	7414.0
178.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264