




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
Data File : VV029971.D
Acq On : 27 Jan 2023 11:38
Operator : SY/MD
Sample : 01315-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B53

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/01/2023
Supervised By :Mahesh Dadoda 02/01/2023

Quant Time: Jan 28 02:22:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jan 28 02:00:30 2023
Response via : Initial Calibration

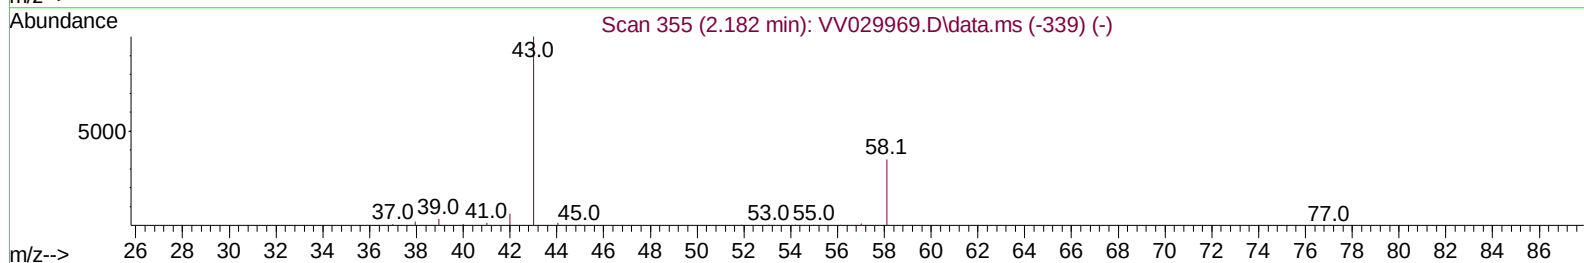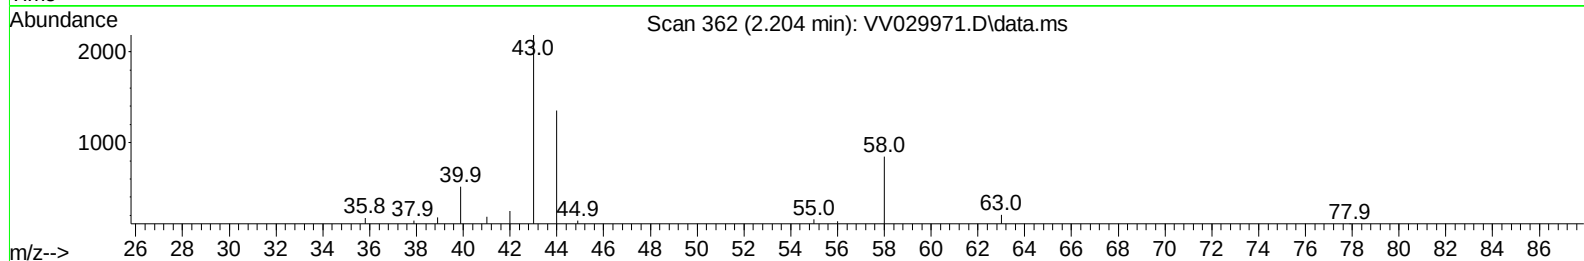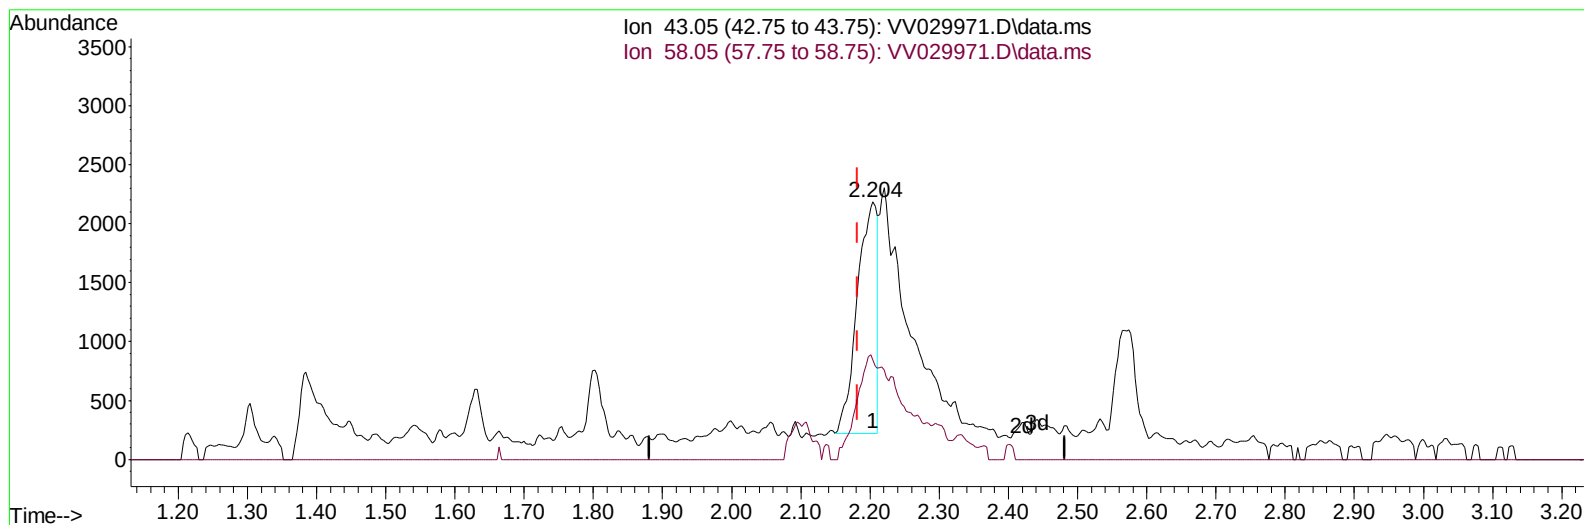

TIC: VV029971.D\data.ms

(13) Acetone (T)

2.204min (+ 0.022) 1.59 ug/L

response 3938

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	103.76#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
 Data File : VV029971.D
 Acq On : 27 Jan 2023 11:38
 Operator : SY/MD
 Sample : 01315-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B53

Manual IntegrationsAPPROVED

Quant Time: Jan 28 02:22:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 28 02:00:30 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

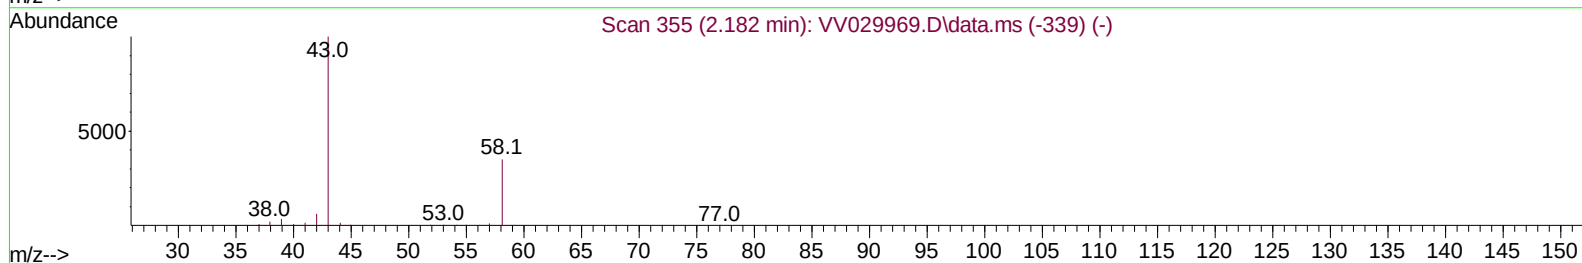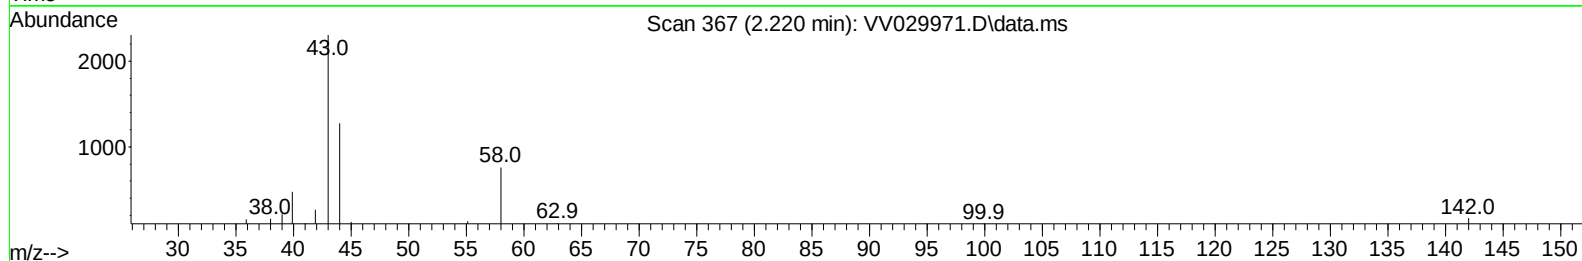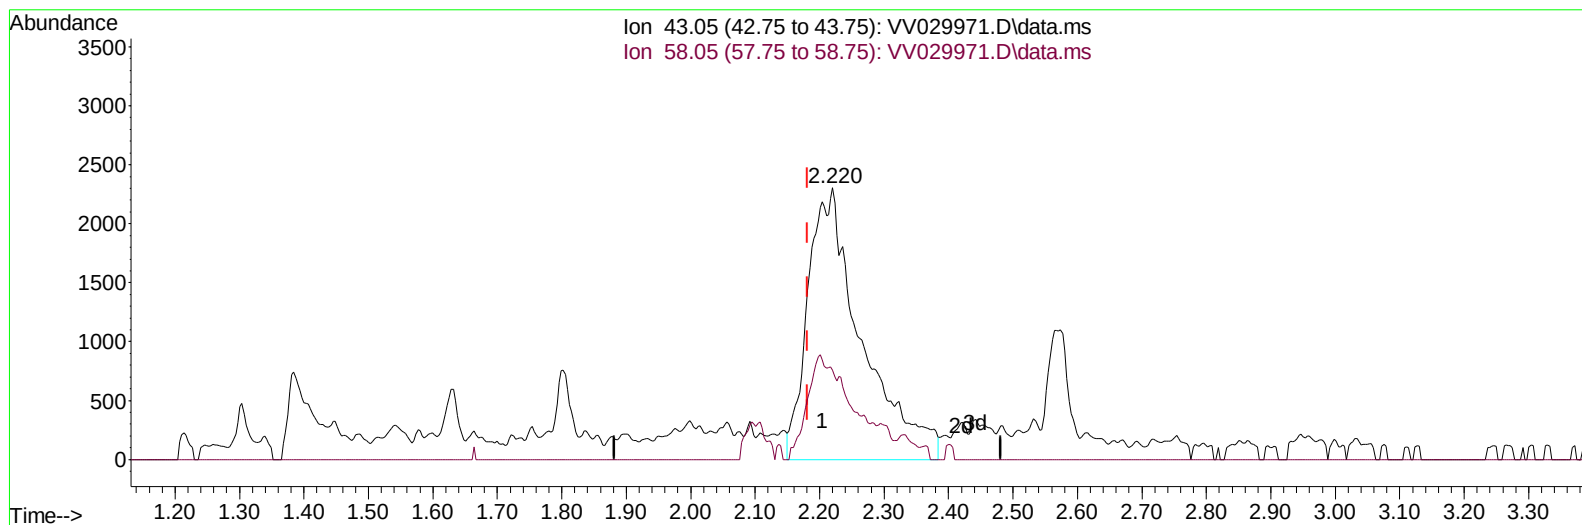

TIC: VV029971.D\data.ms

(13) Acetone (T)

2.220min (+ 0.039) 5.36 ug/L m

response 13268

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	30.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
 Data File : VV029971.D
 Acq On : 27 Jan 2023 11:38
 Operator : SY/MD
 Sample : 01315-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B53

Manual IntegrationsAPPROVED

Quant Time: Jan 28 02:22:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 28 02:00:30 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	257806	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	240753	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	120705	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	84314	4.312	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	86.200%		
7) Chloroethane-d5	1.564	69	74613	4.603	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	92.000%		
11) 1,1-Dichloroethene-d2	2.101	63	110827	3.109	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	62.200%		
20) 2-Butanone-d5	3.902	46	146617	42.303	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	84.600%		
24) Chloroform-d	4.336	84	137727	3.840	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	76.800%		
26) 1,2-Dichloroethane-d4	5.021	65	60823	4.004	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	80.000%		
32) Benzene-d6	5.040	84	292626	4.098	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	82.000%		
36) 1,2-Dichloropropane-d6	6.059	67	92076	4.405	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	88.200%		
41) Toluene-d8	7.307	98	246827	3.733	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	74.600%		
43) trans-1,3-Dichloroprop...	7.612	79	29702	3.891	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	77.800%		
46) 2-Hexanone-d5	8.085	63	133212	42.866	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	85.740%		
56) 1,1,2,2-Tetrachloroeth...	10.204	84	61161	3.993	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	79.800%		
66) 1,2-Dichlorobenzene-d4	11.612	152	89064	4.059	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	81.200%		
Target Compounds						
13) Acetone	2.220	43	13268m	5.364	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
Data File : VV029971.D
Acq On : 27 Jan 2023 11:38
Operator : SY/MD
Sample : 01315-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B53

Manual IntegrationsAPPROVED

Quant Time: Jan 28 02:22:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jan 28 02:00:30 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
Supervised By :Mahesh Dadoda 02/01/2023

