

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
 Data File : VV029972.D
 Acq On : 27 Jan 2023 12:02
 Operator : SY/MD
 Sample : 01315-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B54

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

Quant Time: Jan 28 02:23:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 28 02:00:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	229902	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	220154	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	106150	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	87419	5.013	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.200%	
7) Chloroethane-d5	1.564	69	78811	5.452	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	109.000%	
11) 1,1-Dichloroethene-d2	2.101	63	115219	3.625	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.400%	
20) 2-Butanone-d5	3.912	46	149954	48.517	ug/L	0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.040%	
24) Chloroform-d	4.336	84	147210	4.602	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.000%	
26) 1,2-Dichloroethane-d4	5.024	65	65000	4.798	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.000%	
32) Benzene-d6	5.040	84	309484	4.739	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.800%	
36) 1,2-Dichloropropane-d6	6.059	67	99646	5.214	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.200%	
41) Toluene-d8	7.307	98	258158	4.270	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.400%	
43) trans-1,3-Dichloroprop...	7.612	79	31282	4.482	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.600%	
46) 2-Hexanone-d5	8.085	63	144075	50.700	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.400%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	65007	4.641	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.800%	
66) 1,2-Dichlorobenzene-d4	11.609	152	92474	4.792	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	95.800%	
Target Compounds					Qvalue	
13) Acetone	2.211	43	14483m	6.565	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
Data File : VV029972.D
Acq On : 27 Jan 2023 12:02
Operator : SY/MD
Sample : 01315-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0B54

Quant Time: Jan 28 02:23:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jan 28 02:00:30 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 02/01/2023
Supervised By :Mahesh Dadoda 02/01/2023

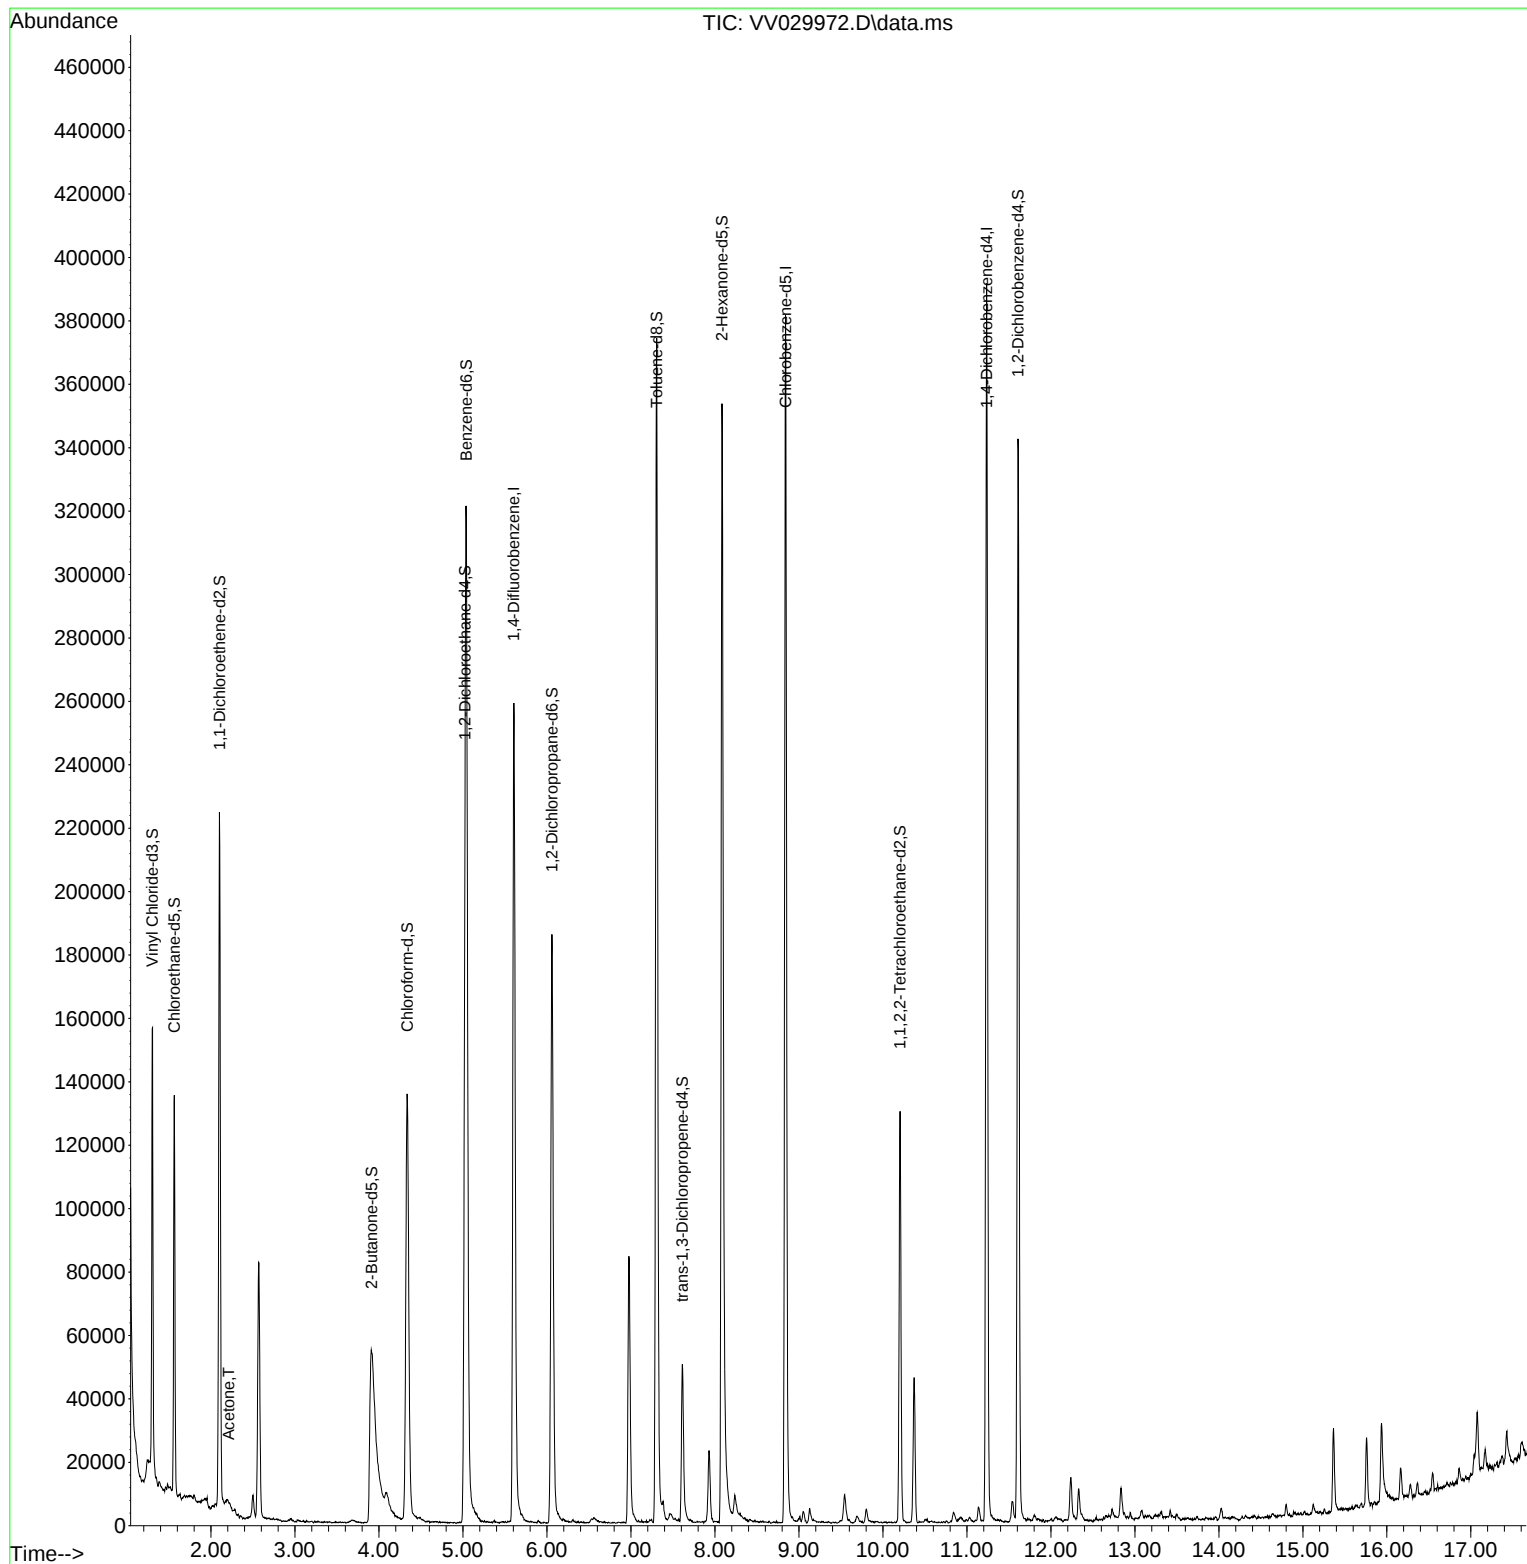

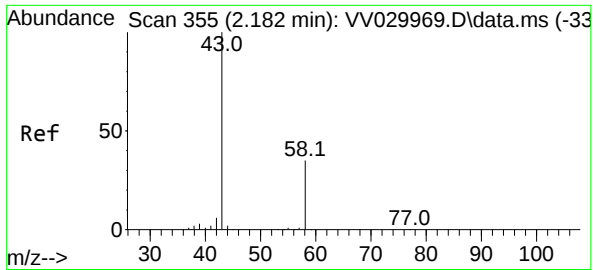

#13
 Acetone
 Concen: 6.565 ug/L m
 RT: 2.211 min Scan# 30
 Delta R.T. 0.029 min
 Lab File: VV029972.D
 Acq: 27 Jan 2023 12:02

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B54

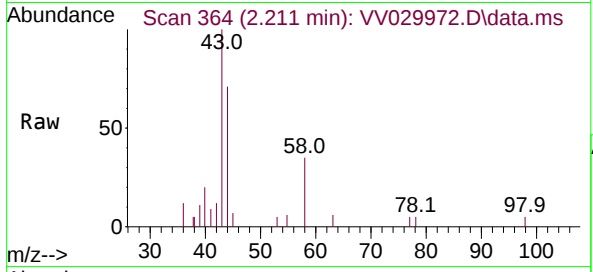

Tgt Ion: 43 Resp: 1448
 Ion Ratio Lower Upper
 43 100
 58 13.8 0.0 68.8

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

