

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012723\
 Data File : VW029975.D
 Acq On : 27 Jan 2023 13:12
 Operator : SY/MD
 Sample : 01315-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0B56

Quant Time: Jan 28 02:24:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 28 02:00:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	227546	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	211451	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	106809	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	83385	4.831	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	96.600%	
7) Chloroethane-d5	1.565	69	76251	5.330	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	106.600%	
11) 1,1-Dichloroethene-d2	2.105	63	109654	3.485	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.800%	
20) 2-Butanone-d5	3.886	46	147811	48.319	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	96.640%	
24) Chloroform-d	4.336	84	138520	4.375	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.600%	
26) 1,2-Dichloroethane-d4	5.021	65	61316	4.573	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
32) Benzene-d6	5.040	84	296486	4.727	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.600%	
36) 1,2-Dichloropropane-d6	6.060	67	93349	5.085	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.800%	
41) Toluene-d8	7.307	98	248926	4.287	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...	7.613	79	29410	4.387	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.800%	
46) 2-Hexanone-d5	8.082	63	125661	46.040	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.080%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	62262	4.628	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	11.612	152	88767	4.571	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	91.400%	


Target Compounds						Qvalue
13) Acetone	2.179	43	23933	10.962	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
 Data File : VV029975.D
 Acq On : 27 Jan 2023 13:12
 Operator : SY/MD
 Sample : 01315-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B56

Quant Time: Jan 28 02:24:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 28 02:00:30 2023
 Response via : Initial Calibration

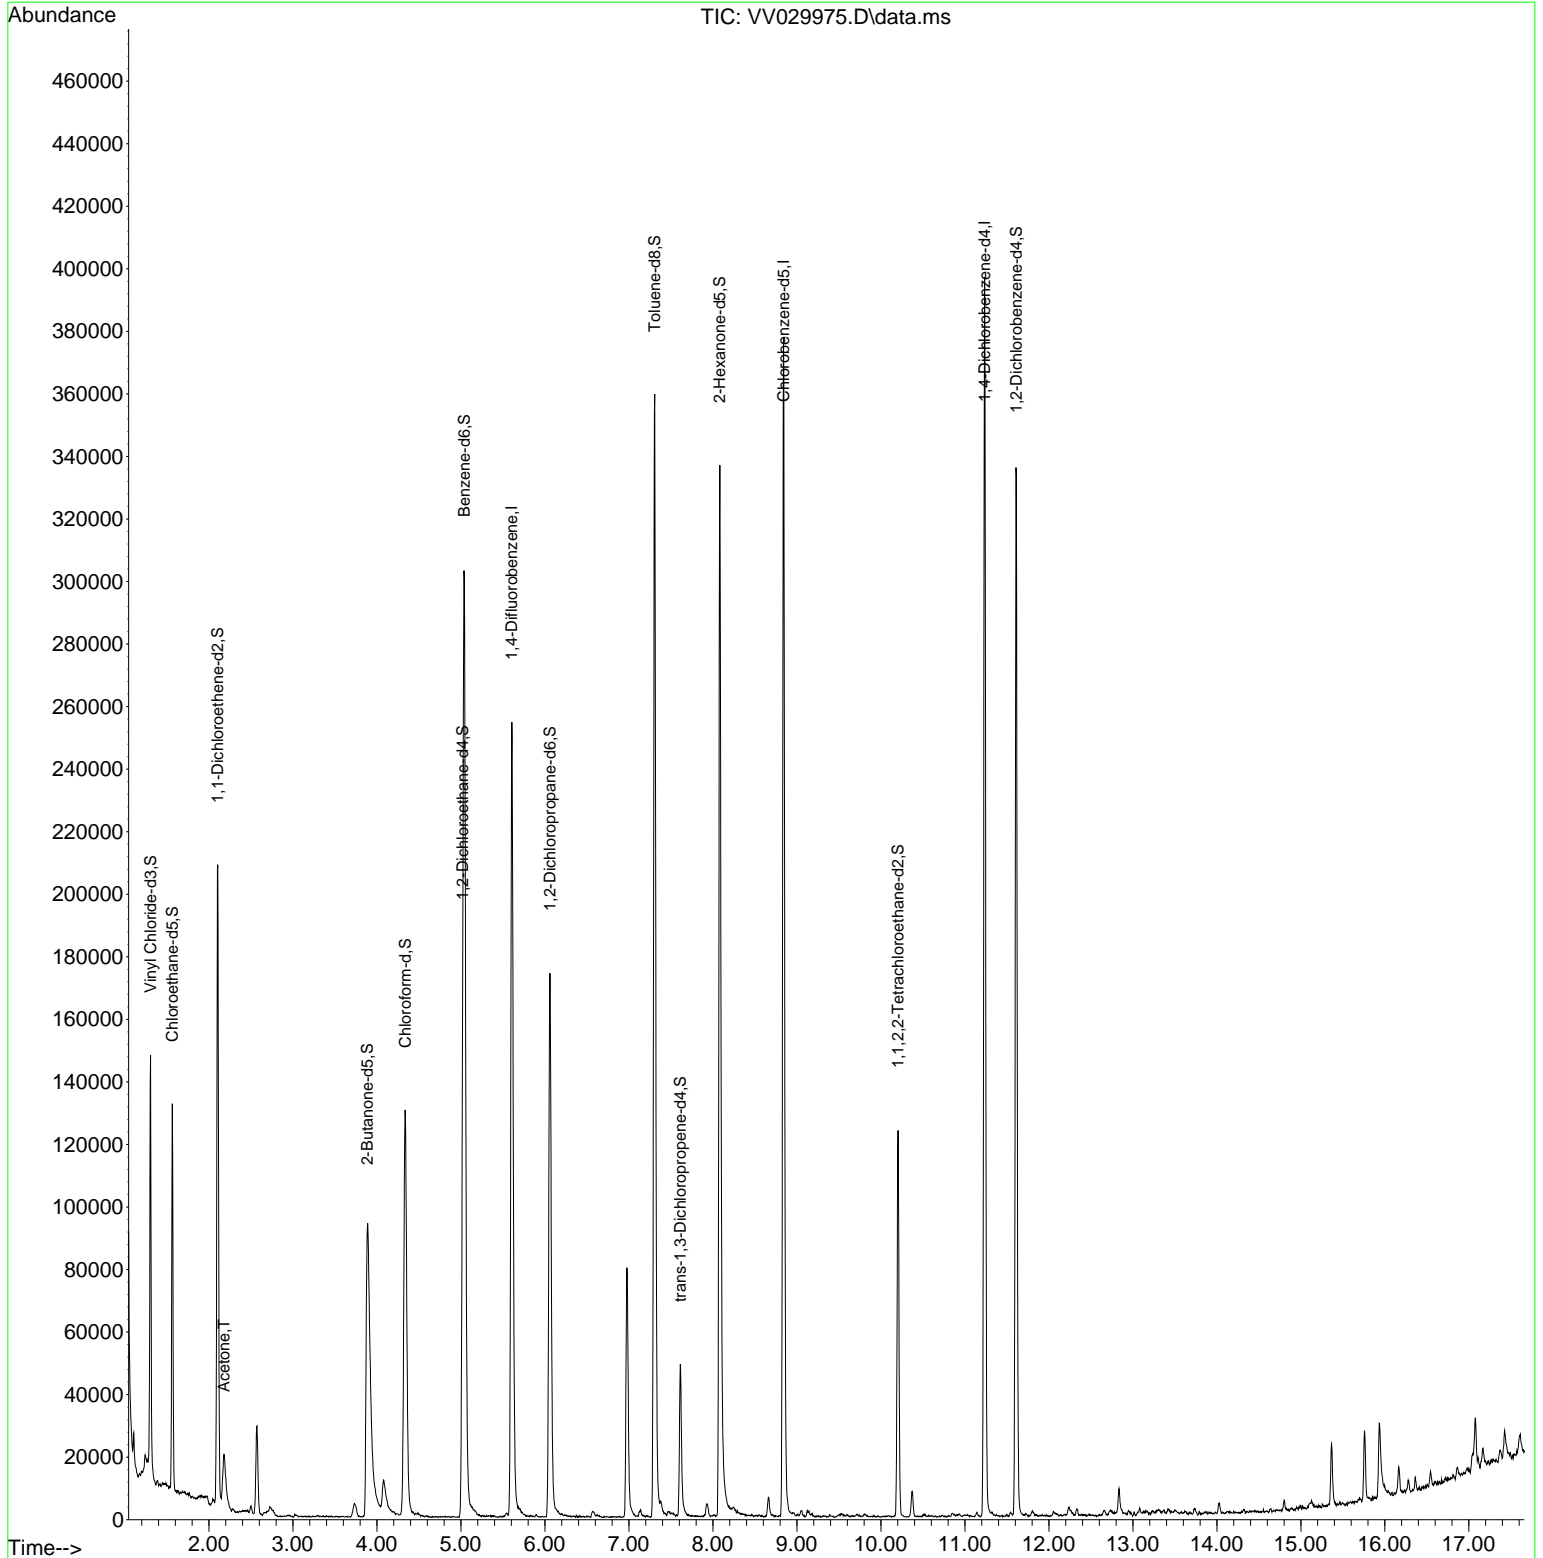

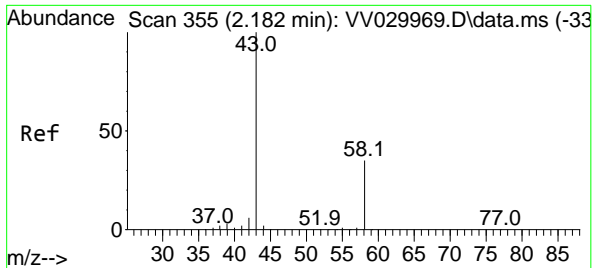

#13
 Acetone
 Concen: 10.962 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV029975.D
 Acq: 27 Jan 2023 13:12

Instrument : MSVOA_V
 ClientSampleId : C0B56

Tgt Ion: 43 Resp: 23933

Ion	Ratio	Lower	Upper
43	100		
58	37.4	0.0	68.8

