

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012723\
 Data File : VW029978.D
 Acq On : 27 Jan 2023 14:34
 Operator : SY/MD
 Sample : 01295-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Quant Time: Jan 28 02:24:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 28 02:00:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	227358	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	211476	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	106848	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	86260	5.002	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.000%
7) Chloroethane-d5	1.564	69	78335	5.480	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.600%
11) 1,1-Dichloroethene-d2	2.101	63	115219	3.665	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%
20) 2-Butanone-d5	3.879	46	152684	49.953	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.900%
24) Chloroform-d	4.330	84	144804	4.578	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.018	65	62032	4.630	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
32) Benzene-d6	5.037	84	306555	4.887	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	6.056	67	95027	5.176	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.600%
41) Toluene-d8	7.304	98	250857	4.319	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.400%
43) trans-1,3-Dichloroprop...	7.609	79	29884	4.457	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.079	63	130258	47.719	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.440%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	61889	4.600	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.000%
66) 1,2-Dichlorobenzene-d4	11.609	152	89901	4.628	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%
Target Compounds						
16) Methylene chloride	2.497	84	5946	0.247	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
Data File : VV029978.D
Acq On : 27 Jan 2023 14:34
Operator : SY/MD
Sample : 01295-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Time: Jan 28 02:24:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jan 28 02:00:30 2023
Response via : Initial Calibration

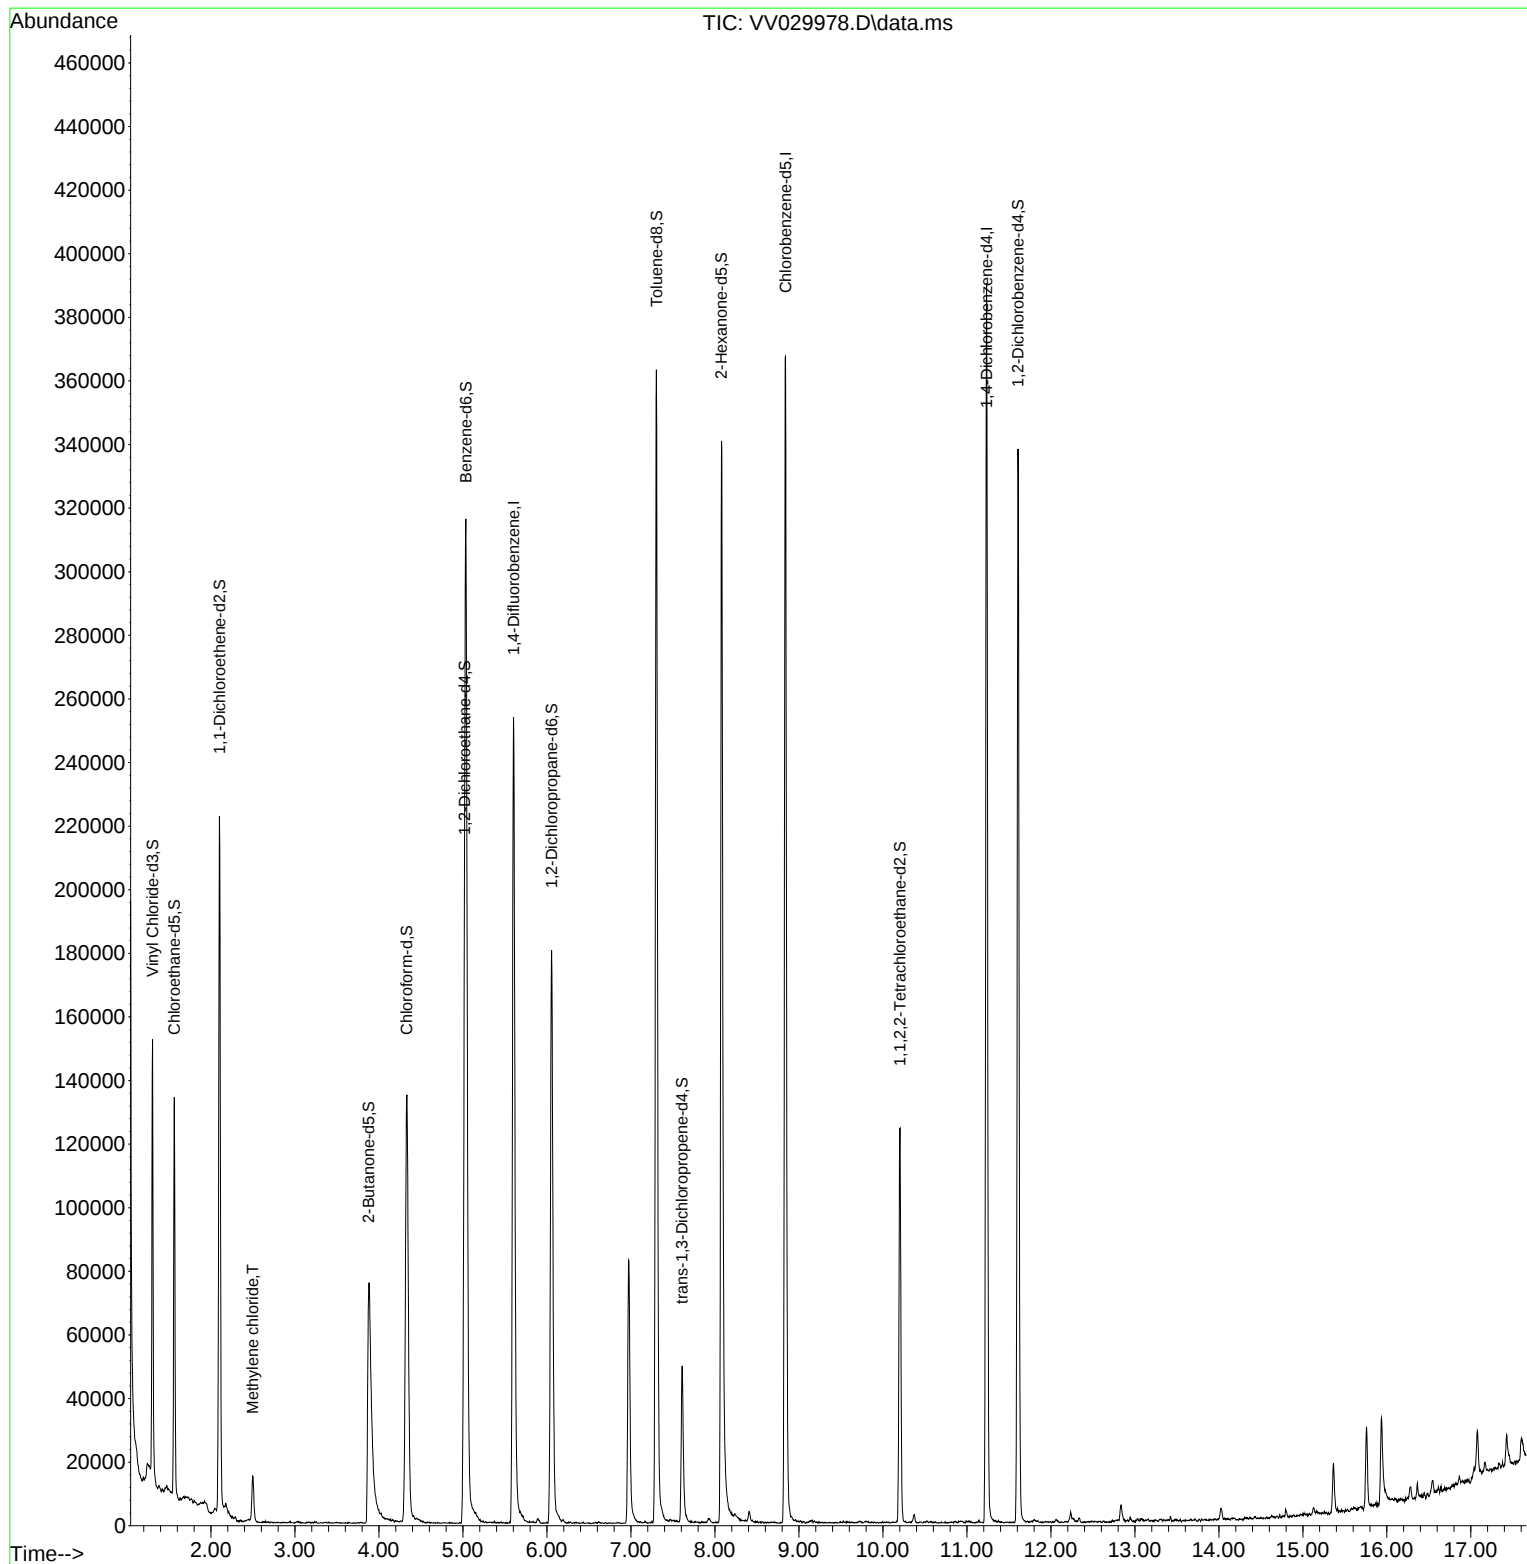

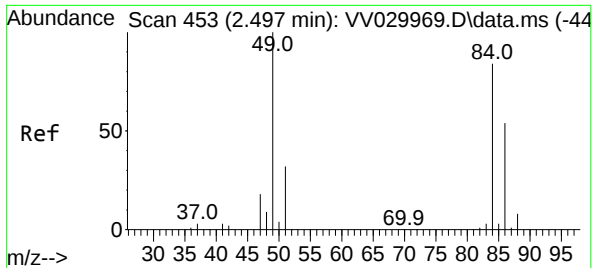

#16
Methylene chloride
Concen: 0.247 ug/L
RT: 2.497 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV029978.D
Acq: 27 Jan 2023 14:34

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Tgt Ion: 84 Resp: 5946
Ion Ratio Lower Upper
84 100
86 65.1 45.0 83.6
49 109.2 71.5 132.7

