


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012723\
Data File : VV029968.D
Acq On : 27 Jan 2023 09:57
Operator : SY/MD
Sample : BFB218
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB218

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jan 28 02:00:30 2023

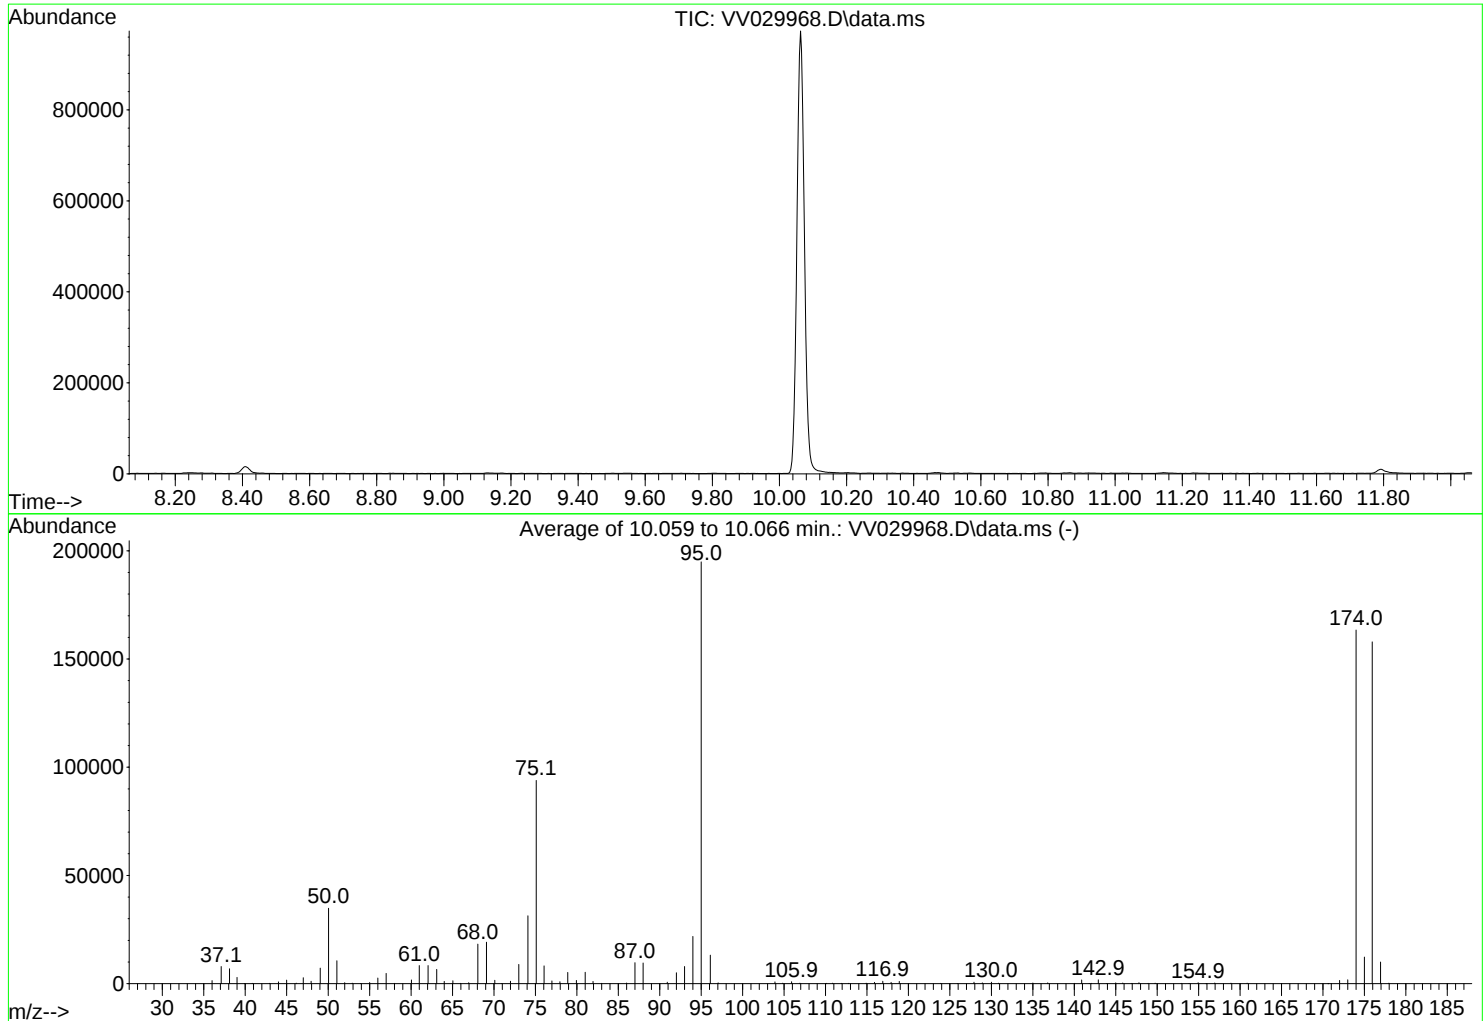

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	34845	PASS
75	95	30	80	48.2	93896	PASS
95	95	100	100	100.0	194901	PASS
96	95	5	9	6.8	13188	PASS
173	174	0.00	2	1.1	1792	PASS
174	95	50	120	83.8	163371	PASS
175	174	5	9	7.5	12280	PASS
176	174	95	105	96.7	157952	PASS
177	176	5	10	6.3	9979	PASS

m/z	Abundance
39.90	369.0
44.00	648.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	1373.0
37.10	7774.0
38.10	6834.0
39.00	2940.0
39.90	412.0
40.80	139.0
42.90	165.0
44.00	1495.0
45.00	1609.0
46.20	253.0
47.00	2859.0
48.00	1130.0
49.10	7047.0
50.00	34800.0
51.10	10639.0
52.00	432.0
52.90	222.0
55.00	611.0
56.00	2569.0
57.00	4712.0
58.00	161.0
60.00	1740.0
61.00	8247.0
62.10	8275.0
63.10	6552.0
64.00	1189.0
65.10	1358.0
66.00	145.0
67.00	487.0
68.10	17952.0
69.10	19128.0
70.10	1559.0
72.00	1113.0
73.00	8844.0
74.10	31168.0
75.10	92064.0
76.00	8136.0
77.00	1198.0
77.90	962.0
78.90	5061.0
79.90	1564.0
81.00	5107.0
82.00	1017.0
83.00	166.0
86.00	233.0
87.00	9407.0
88.00	9631.0
90.90	628.0
92.00	5056.0
93.00	7805.0
94.00	21720.0
95.00	191680.0
96.10	13104.0
97.00	333.0
103.90	891.0
104.80	271.0
105.90	875.0
106.90	170.0
110.10	120.0
110.90	196.0
111.90	145.0
112.70	162.0
114.90	244.0
115.90	546.0
116.90	1084.0
117.90	596.0
118.90	1071.0
123.90	127.0
127.90	572.0
128.90	341.0
130.00	669.0
130.80	188.0
135.00	342.0
136.80	334.0
140.10	183.0
140.90	1697.0
142.00	221.0
142.90	1788.0
144.00	123.0
145.00	443.0
145.80	295.0
146.90	160.0
147.80	501.0
148.90	140.0
149.80	207.0
152.90	139.0
153.90	114.0
155.00	465.0
157.00	288.0
158.80	161.0
160.80	239.0
170.60	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

172.00	1445.0
173.00	1718.0
174.00	156928.0
175.00	11843.0
176.00	150784.0
177.00	9926.0
177.90	250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	1423.0
37.10	8214.0
38.10	7118.0
39.00	2980.0
39.90	460.0
40.80	130.0
42.90	153.0
44.00	1491.0
45.00	1722.0
46.10	234.0
47.00	2778.0
47.90	1118.0
49.10	7412.0
50.10	35992.0
51.10	10931.0
52.00	471.0
52.90	221.0
53.90	121.0
55.00	550.0
56.00	2719.0
57.00	4872.0
58.00	186.0
60.10	1729.0
61.00	8677.0
62.00	8592.0
63.10	6775.0
64.00	1093.0
65.00	1373.0
65.90	158.0
66.90	502.0
68.00	18976.0
69.10	19824.0
70.10	1607.0
70.90	122.0
72.00	1129.0
73.00	9282.0
74.10	32544.0
75.10	96968.0
76.10	8364.0
77.00	1296.0
77.90	963.0
78.90	5293.0
79.90	1511.0
81.00	5433.0
82.00	1034.0
83.00	195.0
86.00	262.0
87.00	10036.0
88.00	9898.0
90.90	687.0
92.00	5237.0
93.00	8100.0
94.00	22536.0
95.00	201984.0
96.10	13628.0
97.10	354.0
103.90	859.0
104.90	264.0
105.90	899.0
106.90	237.0
110.10	128.0
110.80	211.0
111.90	171.0
112.80	147.0
114.90	245.0
115.90	597.0
116.90	1128.0
117.90	657.0
118.90	1031.0
123.90	126.0
125.90	114.0
127.90	664.0
128.90	396.0
130.00	705.0
130.90	211.0
135.00	334.0
136.80	364.0
140.00	182.0
140.90	1773.0
142.10	214.0
142.90	1844.0
144.00	124.0
145.00	424.0
145.80	323.0
147.00	167.0
147.80	487.0
148.90	174.0
149.80	206.0
152.90	132.0
153.80	116.0
154.90	469.0
157.00	311.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

158.90	207.0
160.90	265.0
172.00	1535.0
173.00	1867.0
174.00	168896.0
175.00	12622.0
176.00	163200.0
177.00	10408.0
177.90	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	1391.0
37.10	7812.0
38.10	6727.0
39.00	2742.0
39.90	513.0
40.90	113.0
43.00	163.0
44.00	1394.0
45.00	1520.0
46.10	210.0
47.00	2594.0
47.90	1035.0
49.00	7047.0
50.10	33744.0
51.00	10131.0
52.00	408.0
52.90	193.0
53.90	123.0
55.00	485.0
56.00	2588.0
57.00	4553.0
58.00	191.0
60.10	1580.0
61.00	8191.0
62.00	8113.0
63.10	6381.0
64.00	923.0
65.00	1350.0
65.90	157.0
66.90	466.0
68.00	17928.0
69.10	18552.0
70.10	1431.0
71.00	116.0
72.00	1002.0
73.00	8525.0
74.10	30400.0
75.10	92656.0
76.10	8040.0
77.00	1276.0
78.00	854.0
78.90	5130.0
80.00	1333.0
81.00	5182.0
81.90	997.0
83.00	189.0
86.00	302.0
87.00	9693.0
88.00	8987.0
90.90	687.0
92.00	4909.0
93.00	7818.0
94.00	21168.0
95.00	191040.0
96.10	12832.0
97.10	371.0
103.90	769.0
104.90	238.0
105.90	829.0
106.90	274.0
110.10	118.0
110.80	182.0
111.90	174.0
112.90	124.0
114.90	238.0
115.90	571.0
116.90	1068.0
117.90	617.0
118.90	938.0
123.90	117.0
125.90	122.0
127.90	696.0
128.90	409.0
130.00	678.0
130.90	205.0
135.00	275.0
136.80	318.0
140.00	160.0
140.90	1586.0
141.80	185.0
142.90	1811.0
143.90	107.0
145.00	356.0
145.90	313.0
147.00	149.0
147.80	419.0
148.90	187.0
149.70	214.0
152.90	127.0
153.80	106.0
154.90	450.0
155.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

156.90	299.0
159.00	227.0
160.90	271.0
171.00	145.0
172.00	1516.0
173.00	1792.0
174.00	164288.0
175.00	12375.0
175.90	159872.0
176.90	9604.0
178.00	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218