
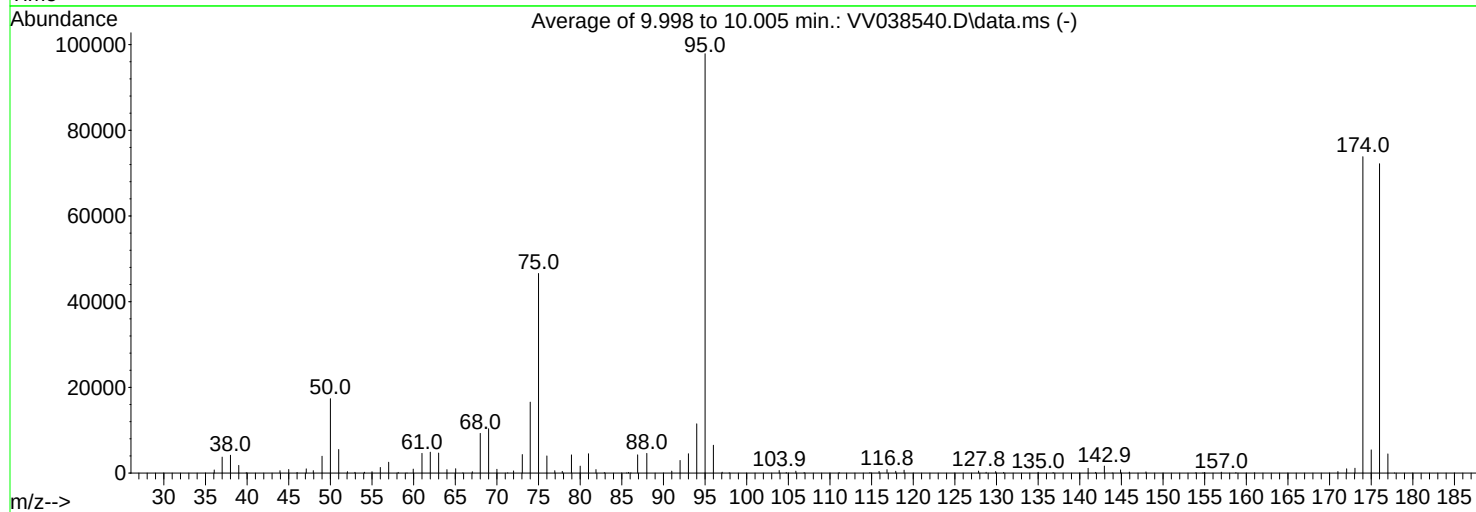


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012725\
Data File : VV038540.D
Acq On : 27 Jan 2025 08:03
Operator : SY/MD
Sample : BFB228
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB228

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jan 28 08:06:10 2025

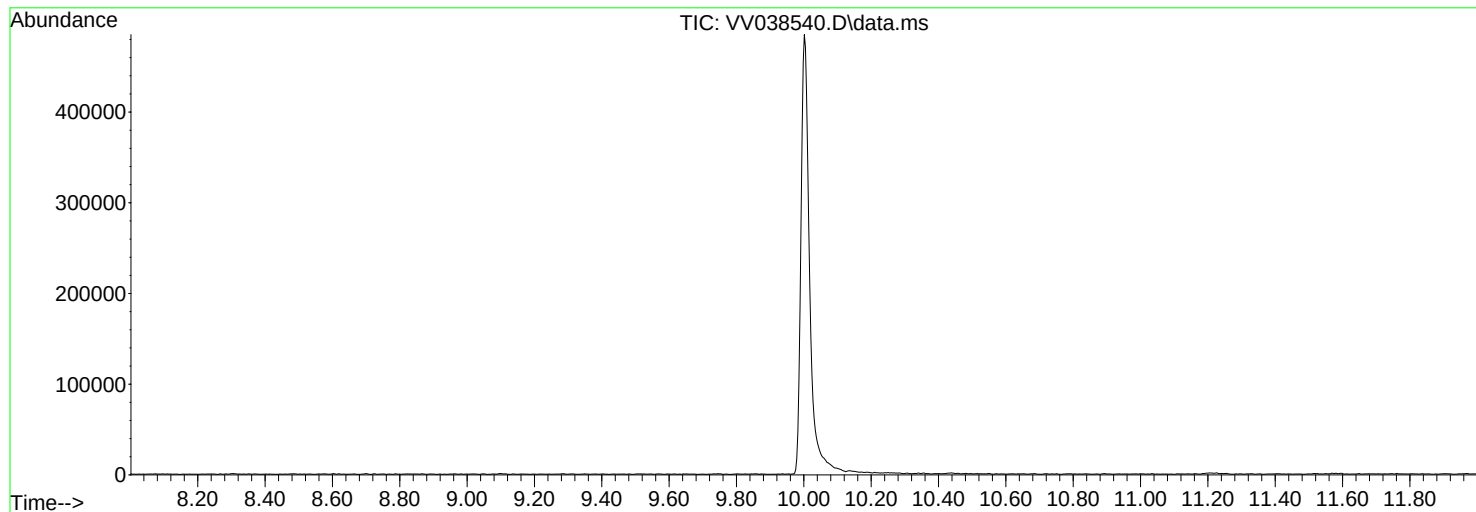

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	17363	PASS
75	95	30	80	47.6	46584	PASS
95	95	100	100	100.0	97872	PASS
96	95	5	9	6.6	6499	PASS
173	174	0.00	2	1.5	1138	PASS
174	95	50	120	75.5	73845	PASS
175	174	5	9	7.3	5419	PASS
176	174	95	101	97.8	72200	PASS
177	176	5	9	6.2	4469	PASS

m/z	Abundance
37.10	133.0
39.90	431.0
44.00	251.0
77.10	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.00	727.0
37.00	3926.0
38.00	3928.0
39.00	1843.0
39.90	586.0
43.90	788.0
45.00	861.0
45.90	153.0
47.20	982.0
47.90	486.0
49.00	3829.0
50.00	17080.0
51.00	5415.0
52.00	290.0
53.00	167.0
54.10	158.0
55.00	314.0
56.00	1319.0
57.00	2414.0
58.10	220.0
59.90	873.0
61.00	4456.0
62.00	5026.0
63.00	4458.0
64.00	814.0
65.00	877.0
67.10	362.0
68.00	9297.0
69.00	10221.0
70.00	922.0
72.00	521.0
73.00	4352.0
74.00	15707.0
75.00	45752.0
76.00	3955.0
76.90	597.0
77.80	457.0
79.00	4154.0
80.00	1526.0
81.00	4280.0
81.90	767.0
82.90	111.0
85.60	146.0
86.10	124.0
86.90	4128.0
88.00	4518.0
91.00	395.0
92.00	2931.0
93.00	4223.0
94.00	11170.0
95.00	94944.0
96.00	6341.0
97.00	247.0
97.90	101.0
103.90	605.0
104.80	131.0
105.80	435.0
106.90	130.0
111.10	116.0
114.90	125.0
115.90	374.0
116.80	727.0
117.90	382.0
118.90	643.0
127.90	465.0
128.80	209.0
129.90	397.0
130.80	115.0
135.00	183.0
136.80	139.0
141.00	1072.0
141.90	189.0
142.90	1550.0
144.90	727.0
145.90	143.0
147.90	309.0
154.00	117.0
154.80	195.0
157.00	177.0
158.90	136.0
171.00	412.0
172.00	903.0
173.10	1091.0
174.00	70464.0
175.00	5382.0
176.00	68856.0
177.00	4129.0
177.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.00	742.0
37.00	3975.0
38.00	4341.0
39.00	1874.0
39.90	556.0
44.00	821.0
45.00	866.0
46.00	138.0
47.10	1000.0
48.00	612.0
49.00	4141.0
50.00	17864.0
51.00	5660.0
52.10	354.0
52.90	182.0
54.10	214.0
55.00	325.0
56.00	1334.0
57.00	2605.0
58.20	179.0
59.20	103.0
60.00	948.0
61.00	4701.0
62.00	5049.0
63.00	4881.0
64.00	828.0
65.00	1052.0
67.10	320.0
68.00	9519.0
69.00	10775.0
70.00	900.0
71.30	124.0
72.00	502.0
73.10	4499.0
74.00	17200.0
75.00	47824.0
76.00	4154.0
76.90	671.0
77.90	419.0
79.00	4342.0
80.00	1725.0
81.00	4703.0
81.90	798.0
82.90	126.0
85.80	187.0
86.90	4387.0
88.00	4789.0
91.00	471.0
92.00	3028.0
93.00	4702.0
94.00	11833.0
95.00	101120.0
96.00	6821.0
97.00	213.0
97.90	125.0
103.90	634.0
104.80	146.0
105.90	456.0
106.90	140.0
111.10	143.0
114.80	147.0
115.90	392.0
116.90	832.0
117.90	418.0
118.90	693.0
127.90	469.0
128.70	185.0
129.90	357.0
130.90	150.0
135.00	206.0
136.80	157.0
141.00	1141.0
141.90	176.0
143.00	1673.0
143.90	106.0
144.90	779.0
146.00	224.0
148.00	299.0
154.00	125.0
155.00	204.0
157.00	217.0
158.70	125.0
171.00	370.0
172.00	1011.0
173.00	1181.0
174.00	76064.0
175.00	5545.0
176.00	74432.0
177.00	4607.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.10	720.0
37.00	3690.0
38.00	4237.0
39.00	1675.0
39.90	457.0
44.00	842.0
45.00	812.0
46.10	187.0
47.00	990.0
48.00	634.0
49.00	3842.0
50.00	17144.0
51.00	5442.0
52.10	365.0
52.90	191.0
54.10	246.0
55.00	325.0
56.00	1295.0
57.00	2582.0
58.20	114.0
60.00	965.0
61.00	4661.0
62.00	4560.0
63.00	4680.0
64.00	783.0
65.10	1122.0
65.90	126.0
67.00	264.0
68.00	8994.0
69.00	10069.0
70.00	840.0
71.30	137.0
72.00	476.0
73.10	4131.0
74.00	16768.0
75.00	46176.0
76.00	3901.0
77.00	732.0
77.90	321.0
78.90	4257.0
80.00	1614.0
81.00	4570.0
81.90	904.0
82.90	124.0
85.80	280.0
86.90	4256.0
88.00	4475.0
91.00	511.0
92.00	2886.0
93.00	4635.0
94.00	11493.0
95.00	97552.0
96.00	6334.0
97.10	176.0
103.90	576.0
104.70	146.0
106.00	452.0
106.90	130.0
111.10	149.0
114.70	149.0
115.90	407.0
116.90	852.0
117.90	493.0
118.90	714.0
127.80	500.0
128.70	181.0
129.90	333.0
130.90	206.0
135.00	204.0
136.80	147.0
141.00	1110.0
141.90	136.0
143.00	1704.0
144.90	753.0
146.00	300.0
147.90	225.0
153.90	111.0
155.00	253.0
157.00	230.0
158.70	145.0
161.00	120.0
171.00	313.0
172.10	1096.0
173.00	1143.0
174.00	75008.0
175.00	5329.0
176.00	73312.0
177.00	4672.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228