

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012820\
 Data File : VV014416.D
 Acq On : 28 Jan 2020 13:06
 Operator : SY/MD
 Sample : VV0128WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK57

Quant Time: Jan 29 10:23:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jan 29 05:25:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	837194	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	775773	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	366239	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	223932	3.82	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.40%
7) Chloroethane-d5	1.58	69	192061	4.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.80%
11) 1,1-Dichloroethene-d2	2.13	63	289122	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	3.95	46	639955	45.48	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.96%
24) Chloroform-d	4.40	84	597554	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
26) 1,2-Dichloroethane-d4	5.08	65	297411	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.09	84	1310780	5.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.20%
36) 1,2-Dichloropropane-d6	6.11	67	420556	5.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	117.20%
41) Toluene-d8	7.35	98	1185903	5.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.20%
43) trans-1,3-Dichloropropene-	7.66	79	153532	4.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.80%
46) 2-Hexanone-d5	8.13	63	718482	53.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.90%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	277183	5.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	396799	5.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.40%


Target Compounds				Ovalue
16) Methylene chloride	2.54	84	27524	0.452 ug/L 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV012820\
Data File : VV014416.D
Acq On : 28 Jan 2020 13:06
Operator : SY/MD
Sample : VV0128WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK57

Quant Time: Jan 29 10:23:05 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jan 29 05:25:35 2020
Response via : Initial Calibration

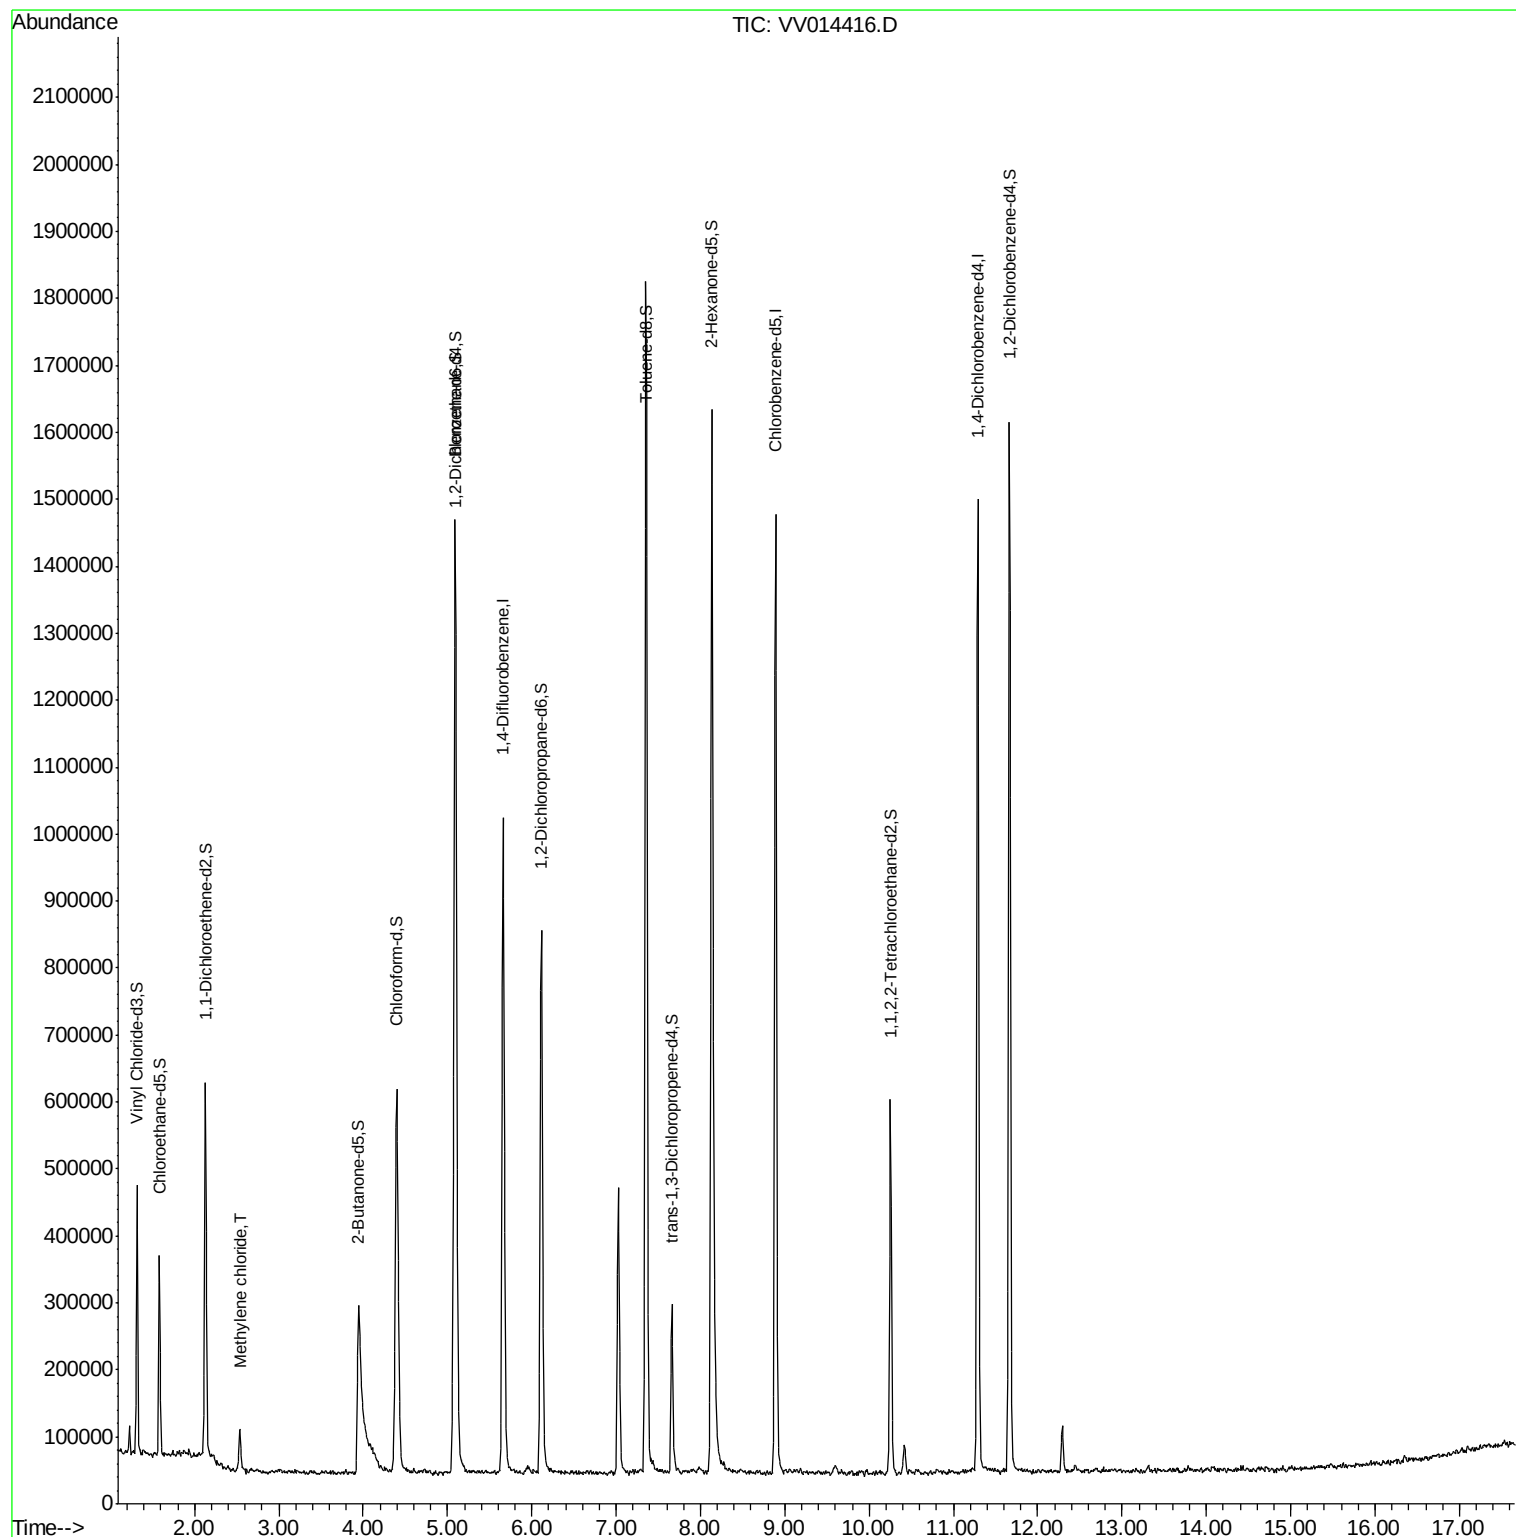

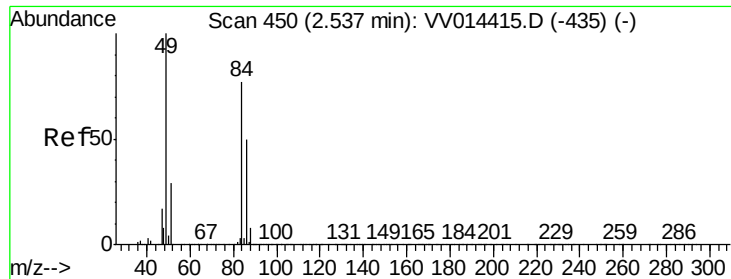

#16
Methylene chloride
Concen: 0.452 ug/L
RT: 2.54 min Scan# 450
Delta R.T. 0.00 min
Lab File: VV014416.D
Acq: 28 Jan 2020 13:06

Instrument :
MSVOA_V
ClientSampleId :
VBLK57

Tot Ion	Ratio	Lower	Upper
84	100		
86	64.8	43.1	80.1
49	116.6	82.1	152.5

