

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020183.D
 Acq On : 27 Jan 2021 10:44
 Operator : SY/MD
 Sample : VSTD00565
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 VSTD00565

Manual Integrations
APPROVED

MMDadoda
 1/29/2021 11:58:33 AM

Quant Time: Jan 27 12:23:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 27 12:22:05 2021
 Response via : Initial Calibration

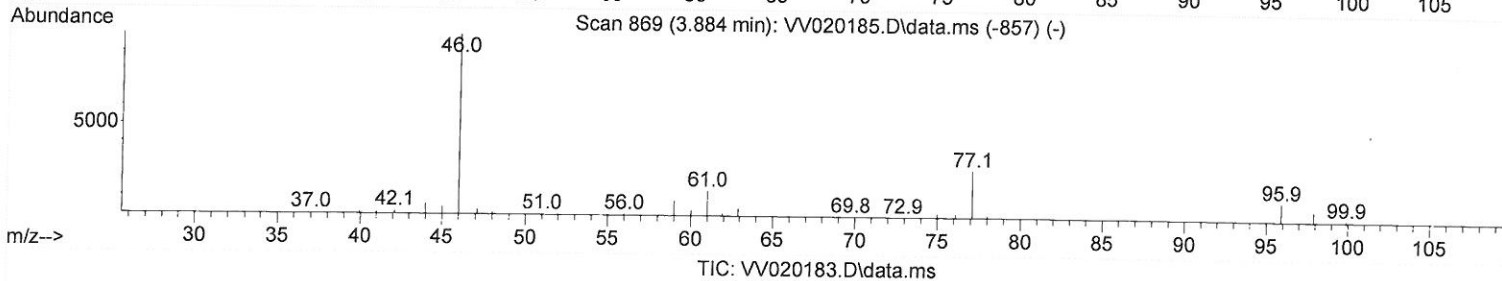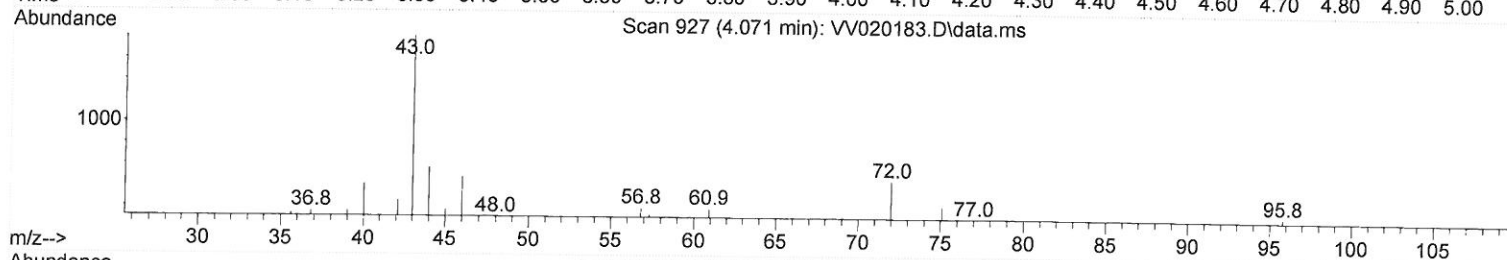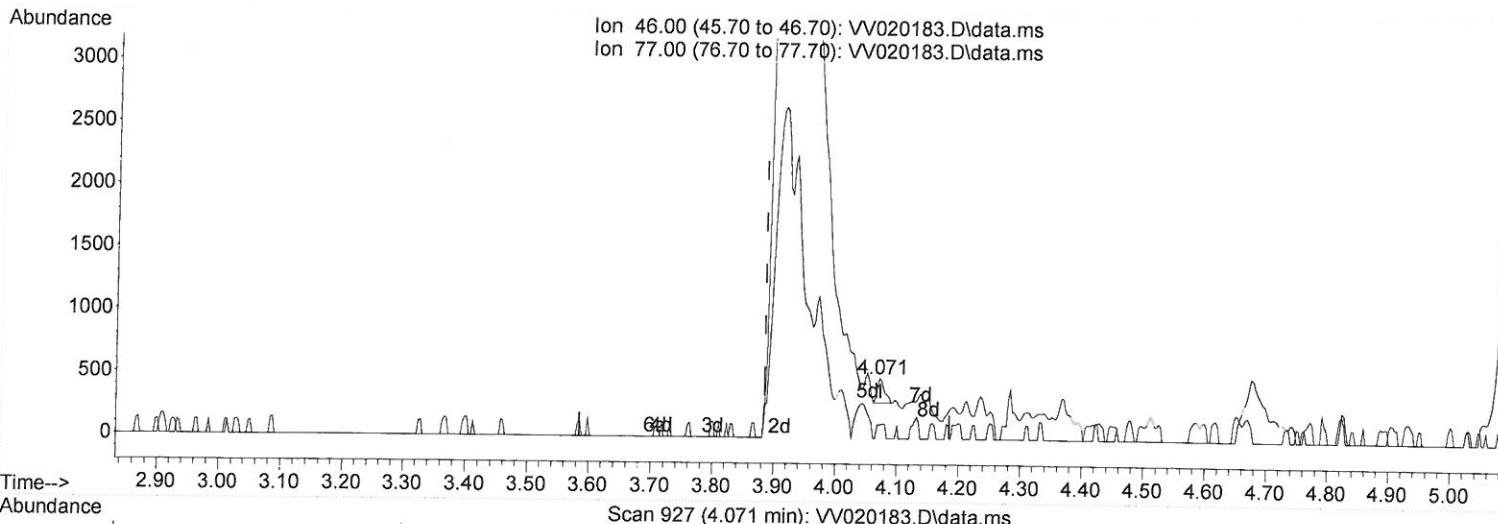

(21) 2-Butanone-d5 (S)

4.071min (+ 0.186) 0.03 ug/L

response 160

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.90	26.25
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020183.D
Acq On : 27 Jan 2021 10:44
Operator : SY/MD
Sample : VSTD00565
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00565

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:58:33 AM

Quant Time: Jan 27 12:23:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 27 12:22:05 2021
Response via : Initial Calibration

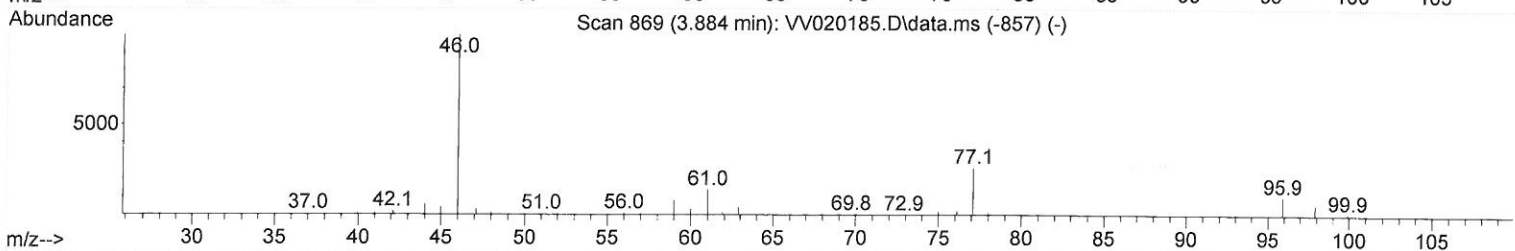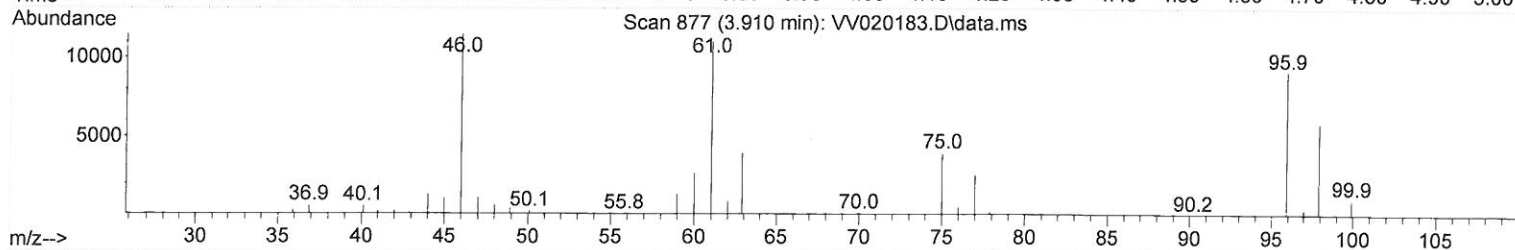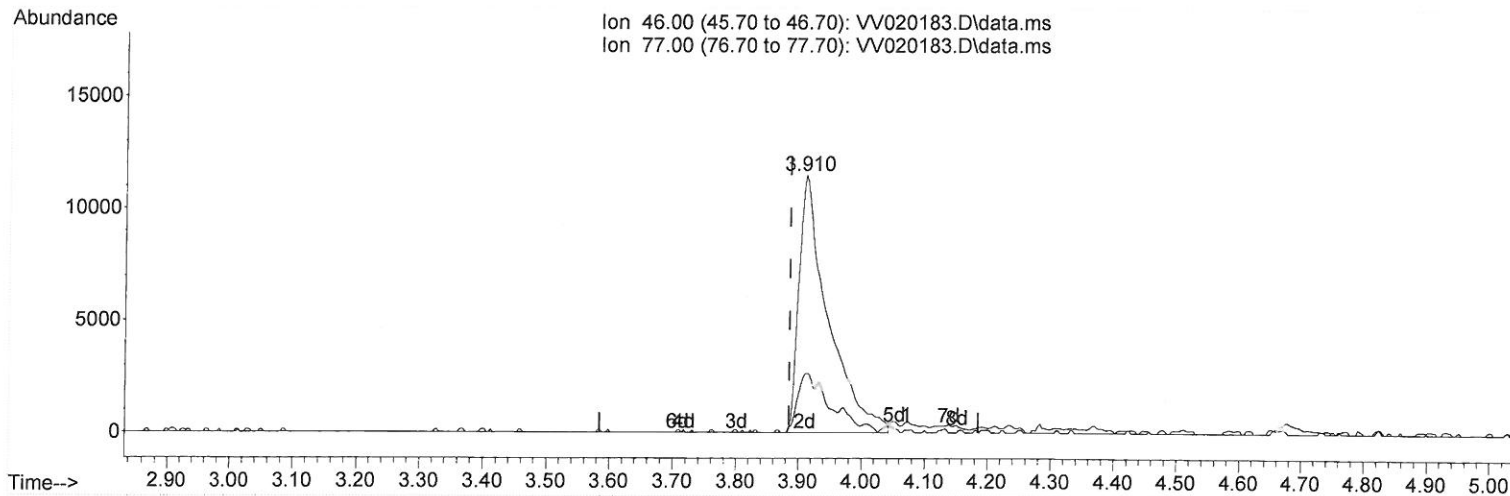

TIC: VV020183.D\data.ms

(21) 2-Butanone-d5 (S)

3.910min (+ 0.026) 7.82 ug/L m

response 36921

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.90	0.11#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020183.D
Acq On : 27 Jan 2021 10:44
Operator : SY/MD
Sample : VSTD00565
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00565

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:58:33 AM

Quant Time: Jan 27 12:23:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 27 12:22:05 2021
Response via : Initial Calibration

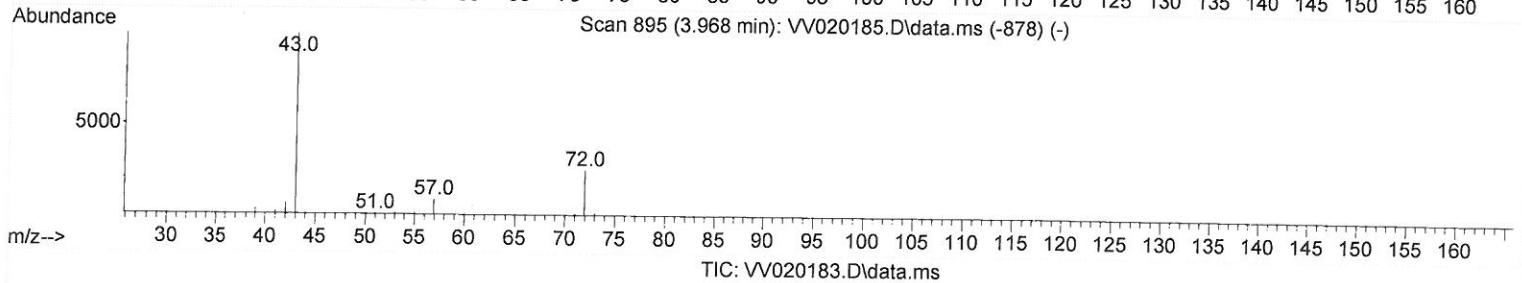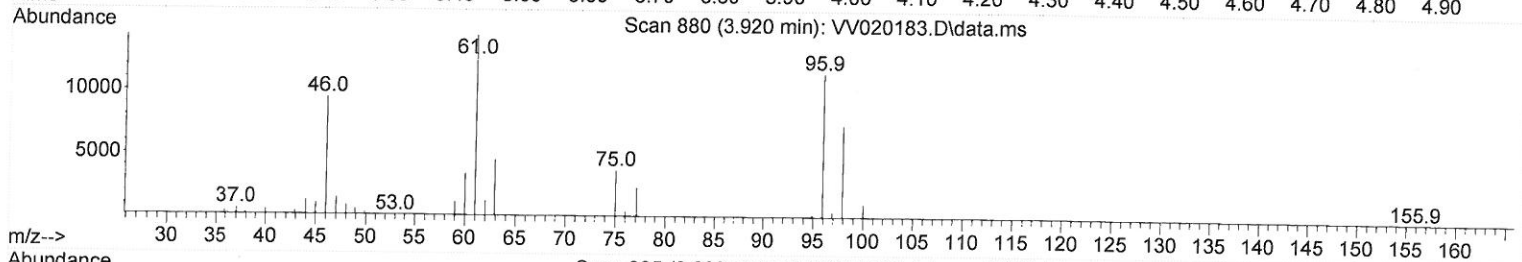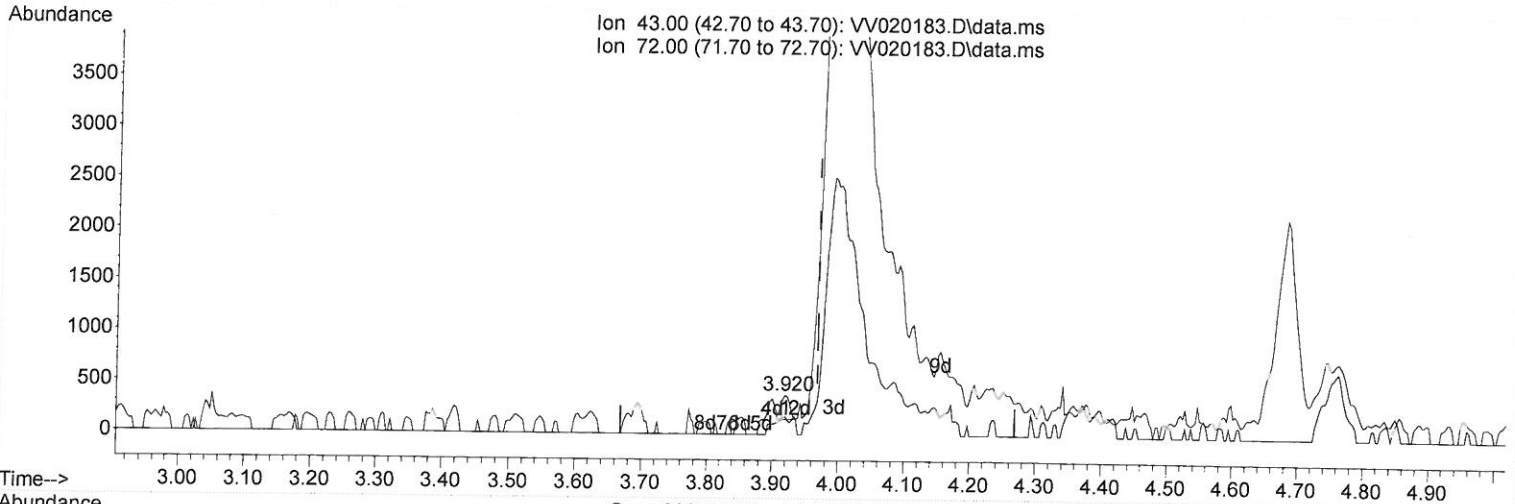

(22) 2-Butanone (T)

3.920min (-0.048) 0.04 ug/L

response 210

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.40	13.81
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020183.D
 Acq On : 27 Jan 2021 10:44
 Operator : SY/MD
 Sample : VSTD00565
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD00565

Manual Integrations
 APPROVED

MMDadoda
 1/29/2021 11:58:33 AM

Quant Time: Jan 27 12:23:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 27 12:22:05 2021
 Response via : Initial Calibration

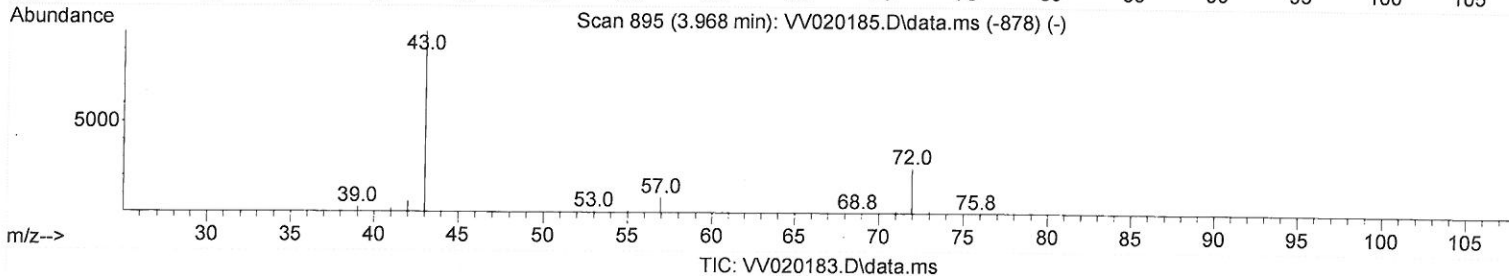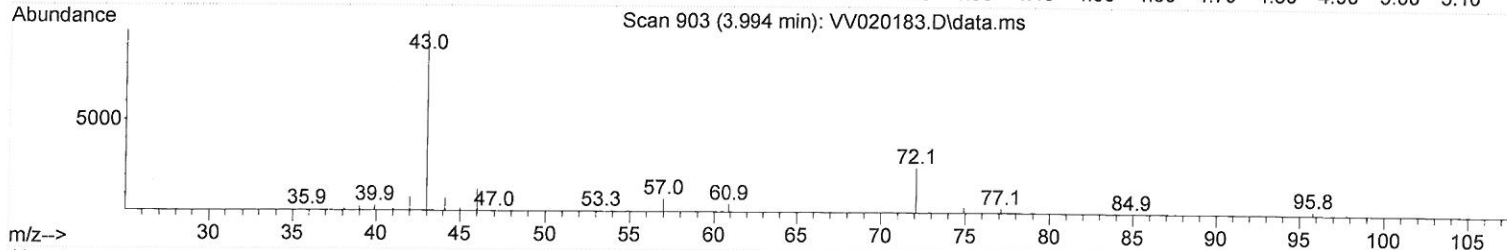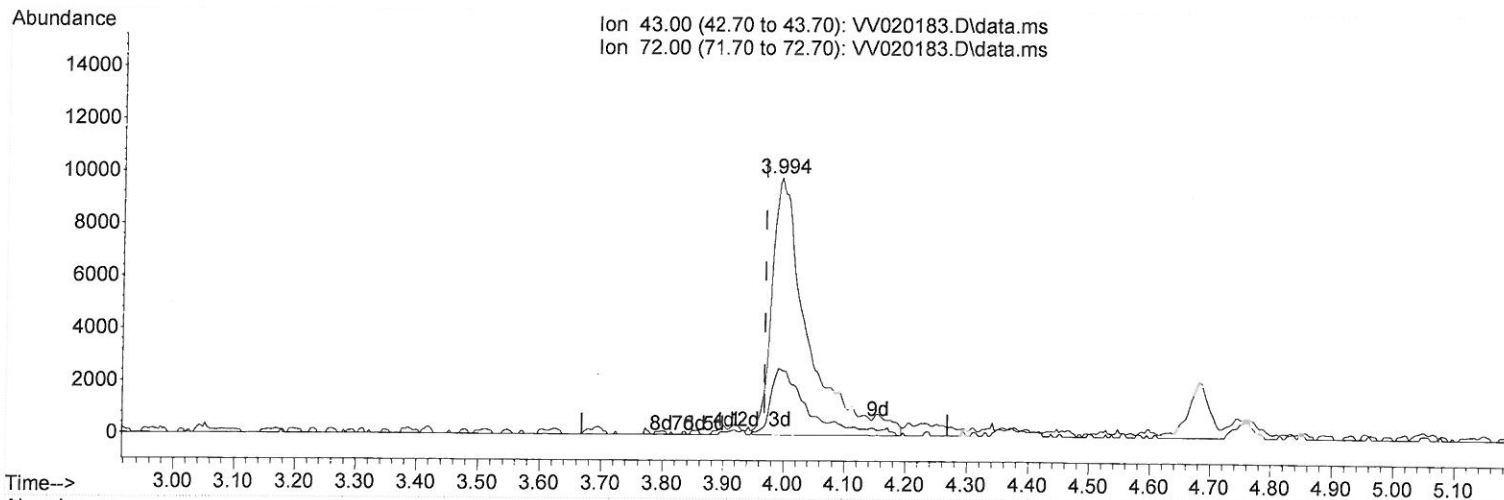

(22) 2-Butanone (T)

3.994min (+ 0.026) 8.01 ug/L m

response 40260

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.40	0.07#
0.00	0.00	0.00
0.00	0.00	0.00

02/02/21 sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020183.D
 Acq On : 27 Jan 2021 10:44
 Operator : SY/MD
 Sample : VSTD00565
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD00565

Manual Integrations
 APPROVED

MMDadoda
 1/29/2021 11:58:33 AM

Quant Time: Jan 27 12:23:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 27 12:22:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.621	114	948156	50.00 ug/L	0.00
28) Chlorobenzene-d5	8.858	117	786335	50.00 ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	473880	50.00 ug/L	0.00
System Monitoring Compounds					
4) Vinyl Chloride-d3	1.309	65	33478	4.71 ug/L	0.00
7) Chloroethane-d5	1.569	69	26373	4.44 ug/L	0.00
11) 1,1-Dichloroethene-d2	2.113	63	54023	4.07 ug/L	0.00
21) 2-Butanone-d5	3.910	46	36921m	7.82 ug/L	0.03
24) Chloroform-d	4.357	84	57808	4.45 ug/L	0.00
26) 1,2-Dichloroethane-d4	5.042	65	37963	4.22 ug/L	0.00
32) Benzene-d6	5.058	84	108497	5.19 ug/L	0.00
36) 1,2-Dichloropropane-d6	6.077	67	33712	5.10 ug/L	0.00
41) Toluene-d8	7.322	98	100705	5.12 ug/L	0.00
43) trans-1,3-Dichloroprop...	7.630	79	14913	4.46 ug/L	0.00
47) 2-Hexanone-d5	8.100	63	26037	9.05 ug/L	0.00
57) 1,1,2,2-Tetrachloroeth...	10.222	84	48516	5.33 ug/L	0.00
64) 1,2-Dichlorobenzene-d4	11.633	152	45830	4.95 ug/L	0.00
Target Compounds					
2) Dichlorodifluoromethane	1.129	85	32735	4.14 ug/L	98
3) Chloromethane	1.241	50	37709	4.72 ug/L	97
5) Vinyl chloride	1.312	62	32385	3.99 ug/L	97
6) Bromomethane	1.524	94	19889	3.97 ug/L	98
8) Chloroethane	1.585	64	20090	3.85 ug/L	91
9) Trichlorofluoromethane	1.756	101	46305	4.00 ug/L	99
10) 1,1,2-Trichloro-1,2,2-...	2.119	101	25301	3.98 ug/L #	87
12) 1,1-Dichloroethene	2.119	96	24781	4.05 ug/L	83
13) Acetone	2.180	43	27877	7.34 ug/L	94
14) Carbon disulfide	2.296	76	71815	3.97 ug/L	99
15) Methyl Acetate	2.438	43	28821	3.89 ug/L	96
16) Methylene chloride	2.511	84	29182	4.29 ug/L	94
17) trans-1,2-Dichloroethene	2.765	96	26998	4.33 ug/L	95
18) Methyl tert-butyl Ether	2.772	73	84001	4.15 ug/L	97
19) 1,1-Dichloroethane	3.196	63	51194	4.30 ug/L	98
20) cis-1,2-Dichloroethene	3.923	96	29091	4.34 ug/L	88
22) 2-Butanone	3.994	43	40260m	8.01 ug/L	
23) Bromochloromethane	4.261	128	15521	4.42 ug/L	88
25) Chloroform	4.383	83	53760	4.29 ug/L	96
27) 1,2-Dichloroethane	5.142	62	43652	4.09 ug/L	98
29) Cyclohexane	4.682	56	40588	4.70 ug/L	95
30) 1,1,1-Trichloroethane	4.614	97	45960	4.92 ug/L #	86
31) Carbon tetrachloride	4.833	117	39479	4.90 ug/L	98
33) Benzene	5.106	78	110035	4.90 ug/L	100
34) Trichloroethene	5.923	95	30225	4.76 ug/L	89
35) Methylcyclohexane	6.135	83	40862	4.51 ug/L	97
37) 1,2-Dichloropropane	6.180	63	26448	4.48 ug/L #	94
38) Bromodichloromethane	6.518	83	37001	4.56 ug/L #	96
39) cis-1,3-Dichloropropene	7.035	75	39911	4.37 ug/L	96
40) 4-Methyl-2-pentanone	7.235	43	73307	8.36 ug/L #	94
42) Toluene	7.396	91	115961	4.82 ug/L	99
44) trans-1,3-Dichloropropene	7.659	75	37020	4.16 ug/L	95

02/02/21 Sy

02/02/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020183.D
 Acq On : 27 Jan 2021 10:44
 Operator : SY/MD
 Sample : VSTD00565
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD00565

Manual Integrations
 APPROVED

MMDadoda
 1/29/2021 11:58:33 AM

Quant Time: Jan 27 12:23:11 2021 .
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 27 12:22:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 1,1,2-Trichloroethane	7.846	97	28481	4.74	ug/L	97
46) Tetrachloroethene	7.981	164	26690	5.28	ug/L	93
48) 2-Hexanone	8.151	43	49557	7.13	ug/L	93
49) Dibromochloromethane	8.254	129	27663	4.25	ug/L	100
50) 1,2-Dibromoethane	8.360	107	27372	4.18	ug/L #	96
51) Chlorobenzene	8.887	112	77105	4.74	ug/L	96
52) Ethylbenzene	9.019	91	108862	4.04	ug/L	96
53) m,p-Xylene	9.145	106	44330	4.49	ug/L	100
54) o-xylene	9.550	106	39316	3.98	ug/L	91
55) Styrene	9.569	104	67533	3.91	ug/L	93
56) Isopropylbenzene	9.939	105	124378	4.67	ug/L	97
58) 1,1,2,2-Tetrachloroethane	10.247	83	45935	5.09	ug/L	97
59) 1,2,3-Trichloropropane	10.280	75	38101	4.81	ug/L	97
61) Bromoform	9.739	173	21274	4.20	ug/L #	98
62) 1,3-Dichlorobenzene	11.190	146	64926	4.51	ug/L	97
63) 1,4-Dichlorobenzene	11.280	146	68905	4.57	ug/L	95
65) 1,2-Dichlorobenzene	11.653	146	65925	4.41	ug/L	93
66) 1,2-Dibromo-3-chloropr...	12.437	75	10236	4.13	ug/L #	77
67) 1,3,5-Trichlorobenzene	12.656	180	53612	4.72	ug/L	97
68) 1,2,4-trichlorobenzene	13.273	180	45434	4.36	ug/L	94
69) Naphthalene	13.511	128	120727	4.00	ug/L	99
70) 1,2,3-Trichlorobenzene	13.755	180	46335	4.49	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\  
Data File : VV020183.D  
Acq On    : 27 Jan 2021  10:44  
Operator  : SY/MD  
Sample    : VSTD00565  
Misc      : 5.0mL/MSVOA_V/WATER  
ALS Vial  : 1   Sample Multiplier: 1
```

Instrument :
MSVOA_V
ClientSampleId :
VSTD00565

Manual Integrations APPROVED

MMDadoda
1/29/2021 11:58:33 AM

Quant Time: Jan 27 12:23:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 27 12:22:05 2021
Response via : Initial Calibration

