

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020198.D
Acq On : 27 Jan 2021 17:44
Operator : SY/MD
Sample : M1201-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z2

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:58:43 AM

Quant Time: Jan 28 05:50:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 28 05:47:43 2021
Response via : Initial Calibration

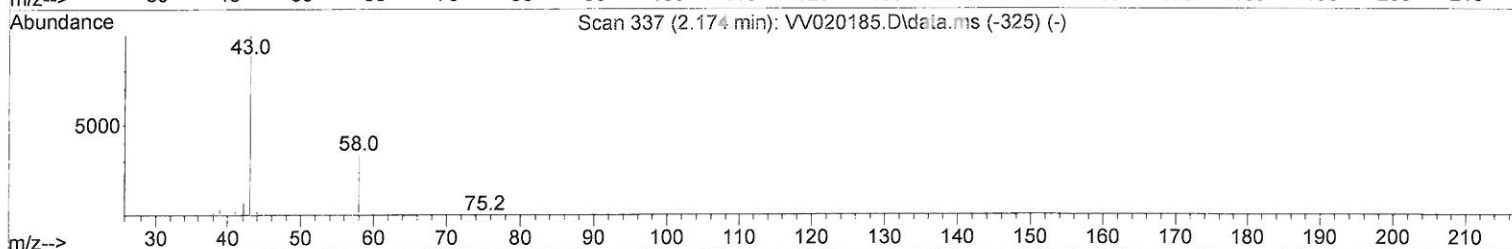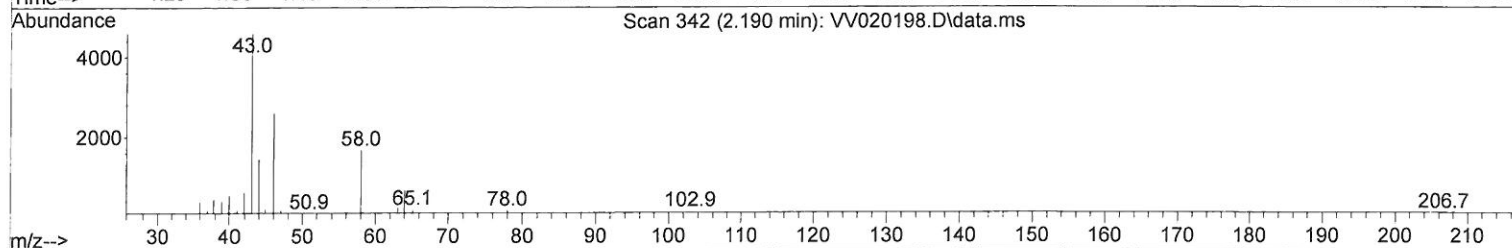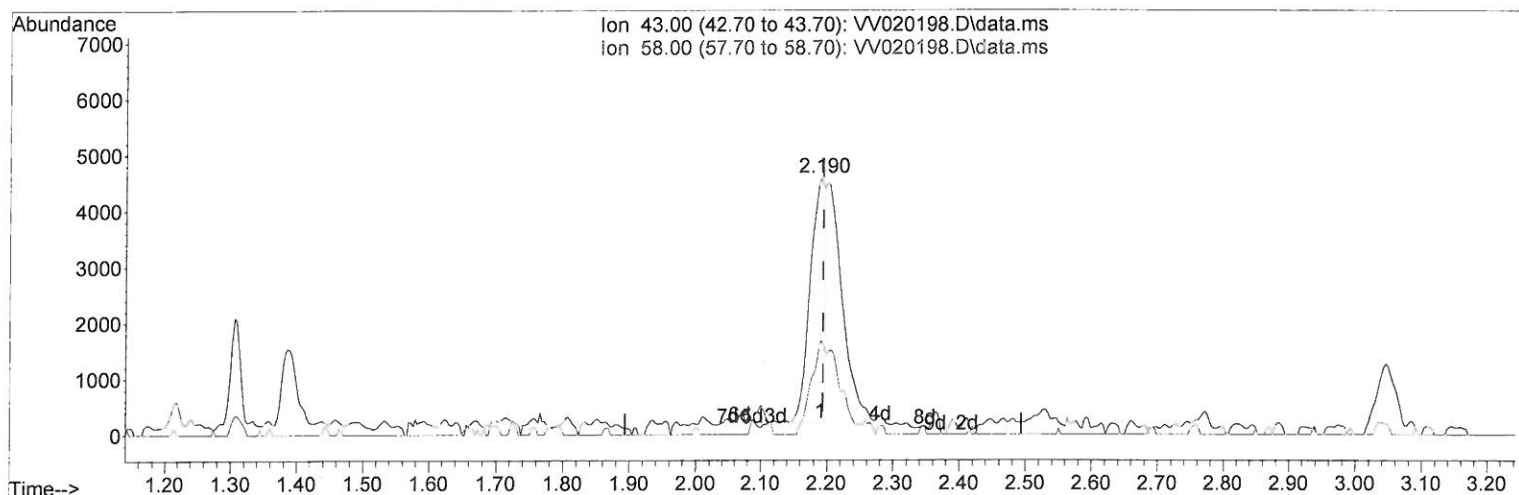

TIC: VV020198.D\data.ms

(13) Acetone (T)

2.190min (-0.003) 2.99 ug/L

response 6931

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.10	38.42
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020198.D
Acq On : 27 Jan 2021 17:44
Operator : SY/MD
Sample : M1201-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z2

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:58:43 AM

Quant Time: Jan 28 05:50:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 28 05:47:43 2021
Response via : Initial Calibration

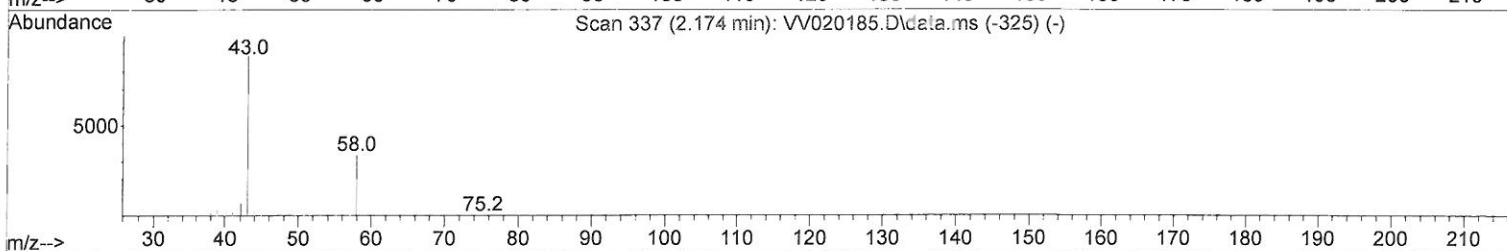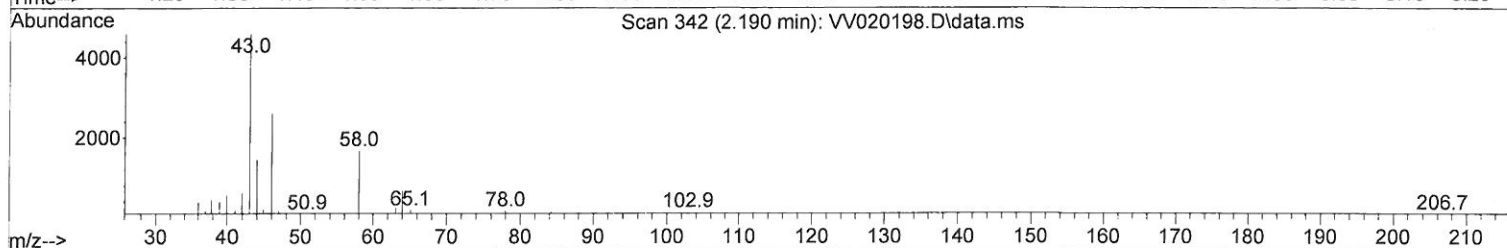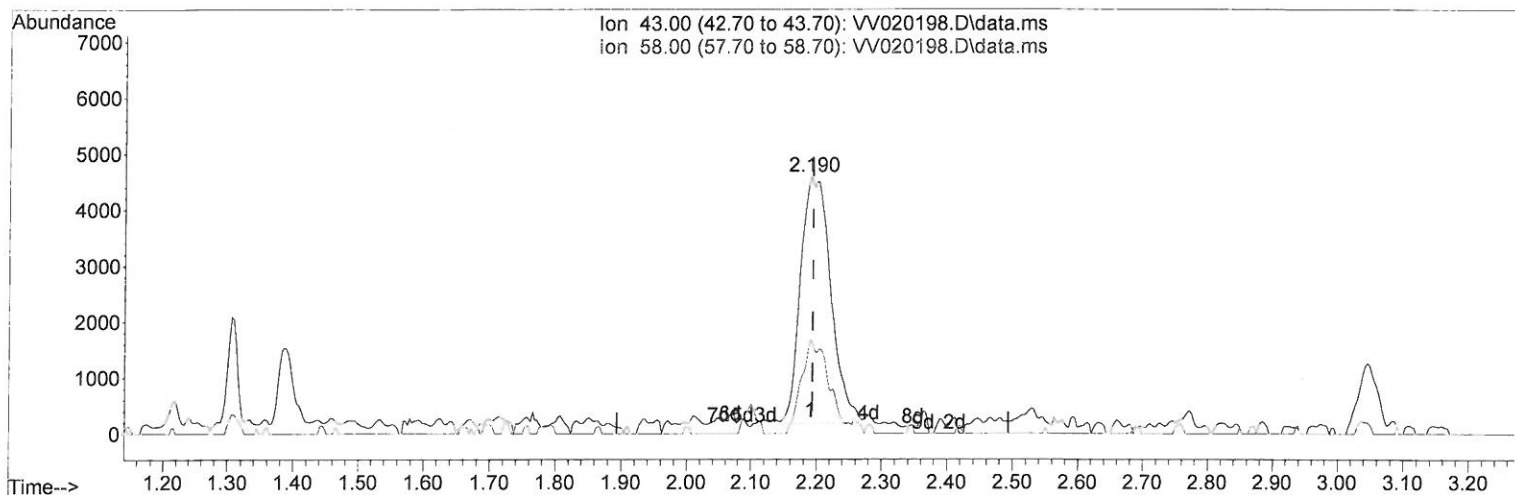

TIC: VV020198.D\data.ms

(13) Acetone (T)

2.190min (-0.003) 6.14 ug/L m

response 14227

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.10	18.72
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020198.D
 Acq On : 27 Jan 2021 17:44
 Operator : SY/MD
 Sample : M1201-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z2

Manual Integrations
 APPROVED

MMDadoda
 1/29/2021 11:58:43 AM

Quant Time: Jan 28 05:50:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 28 05:47:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	917139	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	901733	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.254	152	451529	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.306	65	280870	44.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.18%
7) Chloroethane-d5	1.570	69	197511	40.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.62%
11) 1,1-Dichloroethene-d2	2.107	63	341473	36.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.58%
21) 2-Butanone-d5	3.897	46	389801	96.97	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.97%
24) Chloroform-d	4.354	84	527071	45.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.88%
26) 1,2-Dichloroethane-d4	5.036	65	355229	47.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.74%
32) Benzene-d6	5.055	84	1081425	46.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.68%
36) 1,2-Dichloropropane-d6	6.074	67	332998	46.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.62%
41) Toluene-d8	7.319	98	1034207	47.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.20%
43) trans-1,3-Dichloroprop...	7.624	79	163327	46.35	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.70%
47) 2-Hexanone-d5	8.093	63	287749	90.59	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.59%
57) 1,1,2,2-Tetrachloroeth...	10.222	84	460167	47.13	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.26%
64) 1,2-Dichlorobenzene-d4	11.633	152	449670	52.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.06%

Target Compounds

13) Acetone	2.190	43	14227m	6.14	ug/L	Qvalue
-------------	-------	----	--------	------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

02/02/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020198.D
Acq On : 27 Jan 2021 17:44
Operator : SY/MD
Sample : M1201-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z2

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:58:43 AM

Quant Time: Jan 28 05:50:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 28 05:47:43 2021
Response via : Initial Calibration

