

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020197.D
 Acq On : 27 Jan 2021 17:20
 Operator : SY/MD
 Sample : M1201-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y8

Quant Time: Jan 28 05:50:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 28 05:47:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	933063	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	857891	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.254	152	468686	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	274413	42.34	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.68%	
7) Chloroethane-d5	1.570	69	234528	47.05	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.10%	
11) 1,1-Dichloroethene-d2	2.110	63	333480	35.32	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	70.64%	
21) 2-Butanone-d5	3.891	46	411595	100.64	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	100.64%	
24) Chloroform-d	4.354	84	551185	47.22	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.44%	
26) 1,2-Dichloroethane-d4	5.036	65	380858	50.45	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.90%	
32) Benzene-d6	5.055	84	1090346	49.11	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.22%	
36) 1,2-Dichloropropane-d6	6.074	67	346593	50.67	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	101.34%	
41) Toluene-d8	7.319	98	1014897	49.09	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.18%	
43) trans-1,3-Dichloroprop...	7.627	79	153323	45.73	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.46%	
47) 2-Hexanone-d5	8.090	63	286411	94.77	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	94.77%	
57) 1,1,2,2-Tetrachloroeth...	10.222	84	463131	49.86	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	99.72%	
64) 1,2-Dichlorobenzene-d4	11.630	152	439065	48.94	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.88%	
Target Compounds						
13) Acetone	2.187	43	10175	4.32	ug/L	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020197.D
Acq On : 27 Jan 2021 17:20
Operator : SY/MD
Sample : M1201-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y8


Quant Time: Jan 28 05:50:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 28 05:47:43 2021
Response via : Initial Calibration

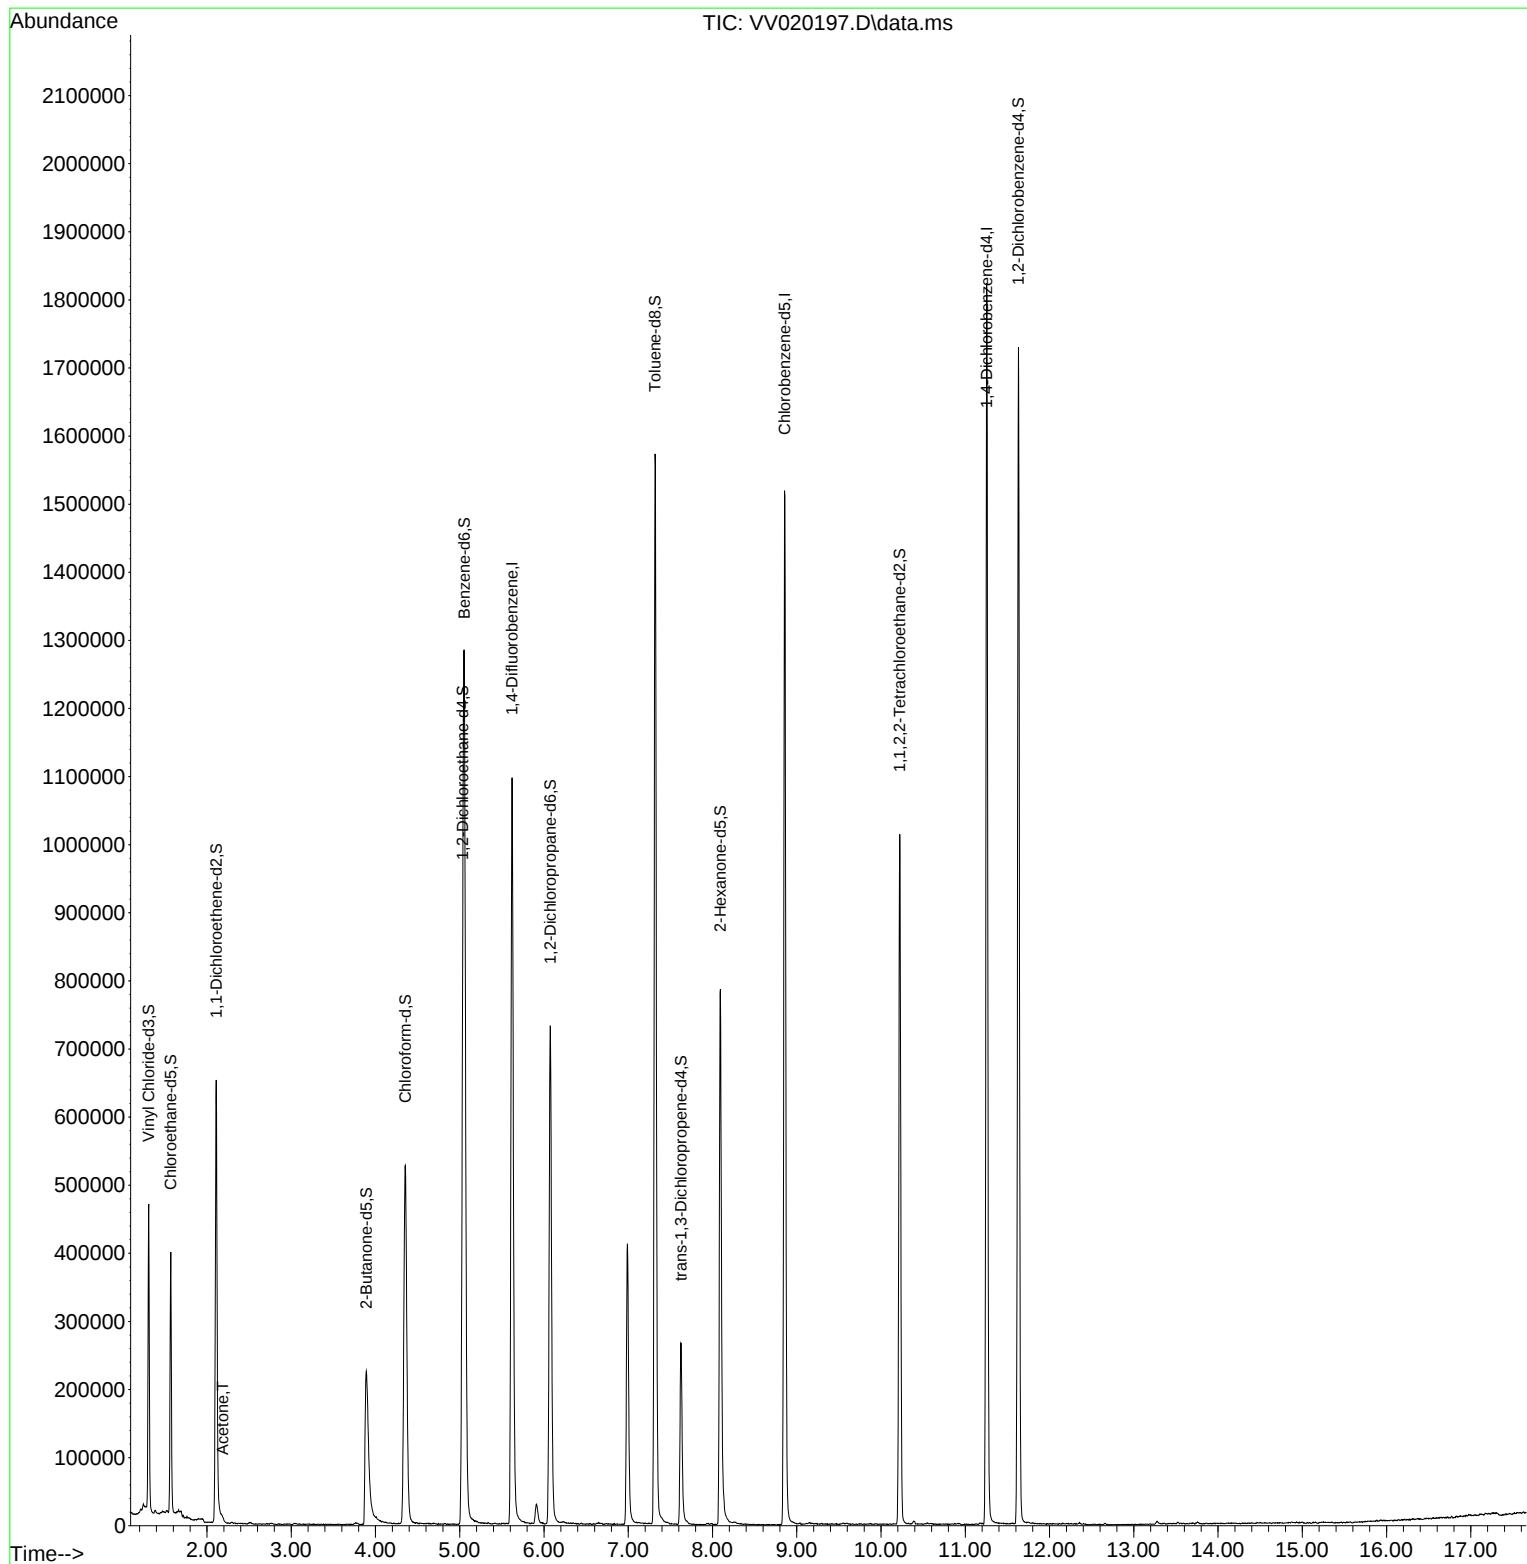

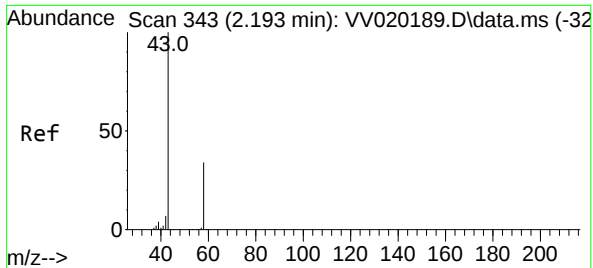

#13
 Acetone
 Concen: 4.32 ug/L
 RT: 2.187 min Scan# 341
 Delta R.T. -0.006 min
 Lab File: VV020197.D
 Acq: 27 Jan 2021 17:20

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y8

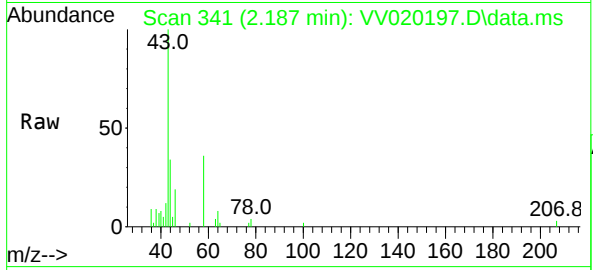

Tgt Ion:	43	Resp:	10175
Ion	Ratio	Lower	Upper
43	100		
58	40.6	0.0	60.2

