

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020200.D
 Acq On : 27 Jan 2021 18:31
 Operator : SY/MD
 Sample : M1258-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z3

Quant Time: Jan 28 05:51:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 28 05:47:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	918400	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	846798	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.254	152	445345	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	273769	42.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.84%
7) Chloroethane-d5	1.569	69	232225	47.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.66%
11) 1,1-Dichloroethene-d2	2.110	63	334585	36.00	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.00%
21) 2-Butanone-d5	3.891	46	405248	100.67	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.67%
24) Chloroform-d	4.354	84	554748	48.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.56%
26) 1,2-Dichloroethane-d4	5.036	65	374481	50.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.80%
32) Benzene-d6	5.055	84	1089548	49.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.44%
36) 1,2-Dichloropropane-d6	6.074	67	344074	50.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.92%
41) Toluene-d8	7.322	98	911250	44.66	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.32%
43) trans-1,3-Dichloroprop...	7.624	79	143086	43.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.48%
47) 2-Hexanone-d5	8.090	63	277498	93.03	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.03%
57) 1,1,2,2-Tetrachloroeth...	10.222	84	462770	50.47	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.94%
64) 1,2-Dichlorobenzene-d4	11.630	152	445034	52.20	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.40%
Target Compounds						
13) Acetone	2.184	43	14257	6.15	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020200.D
Acq On : 27 Jan 2021 18:31
Operator : SY/MD
Sample : M1258-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z3


Quant Time: Jan 28 05:51:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 28 05:47:43 2021
Response via : Initial Calibration

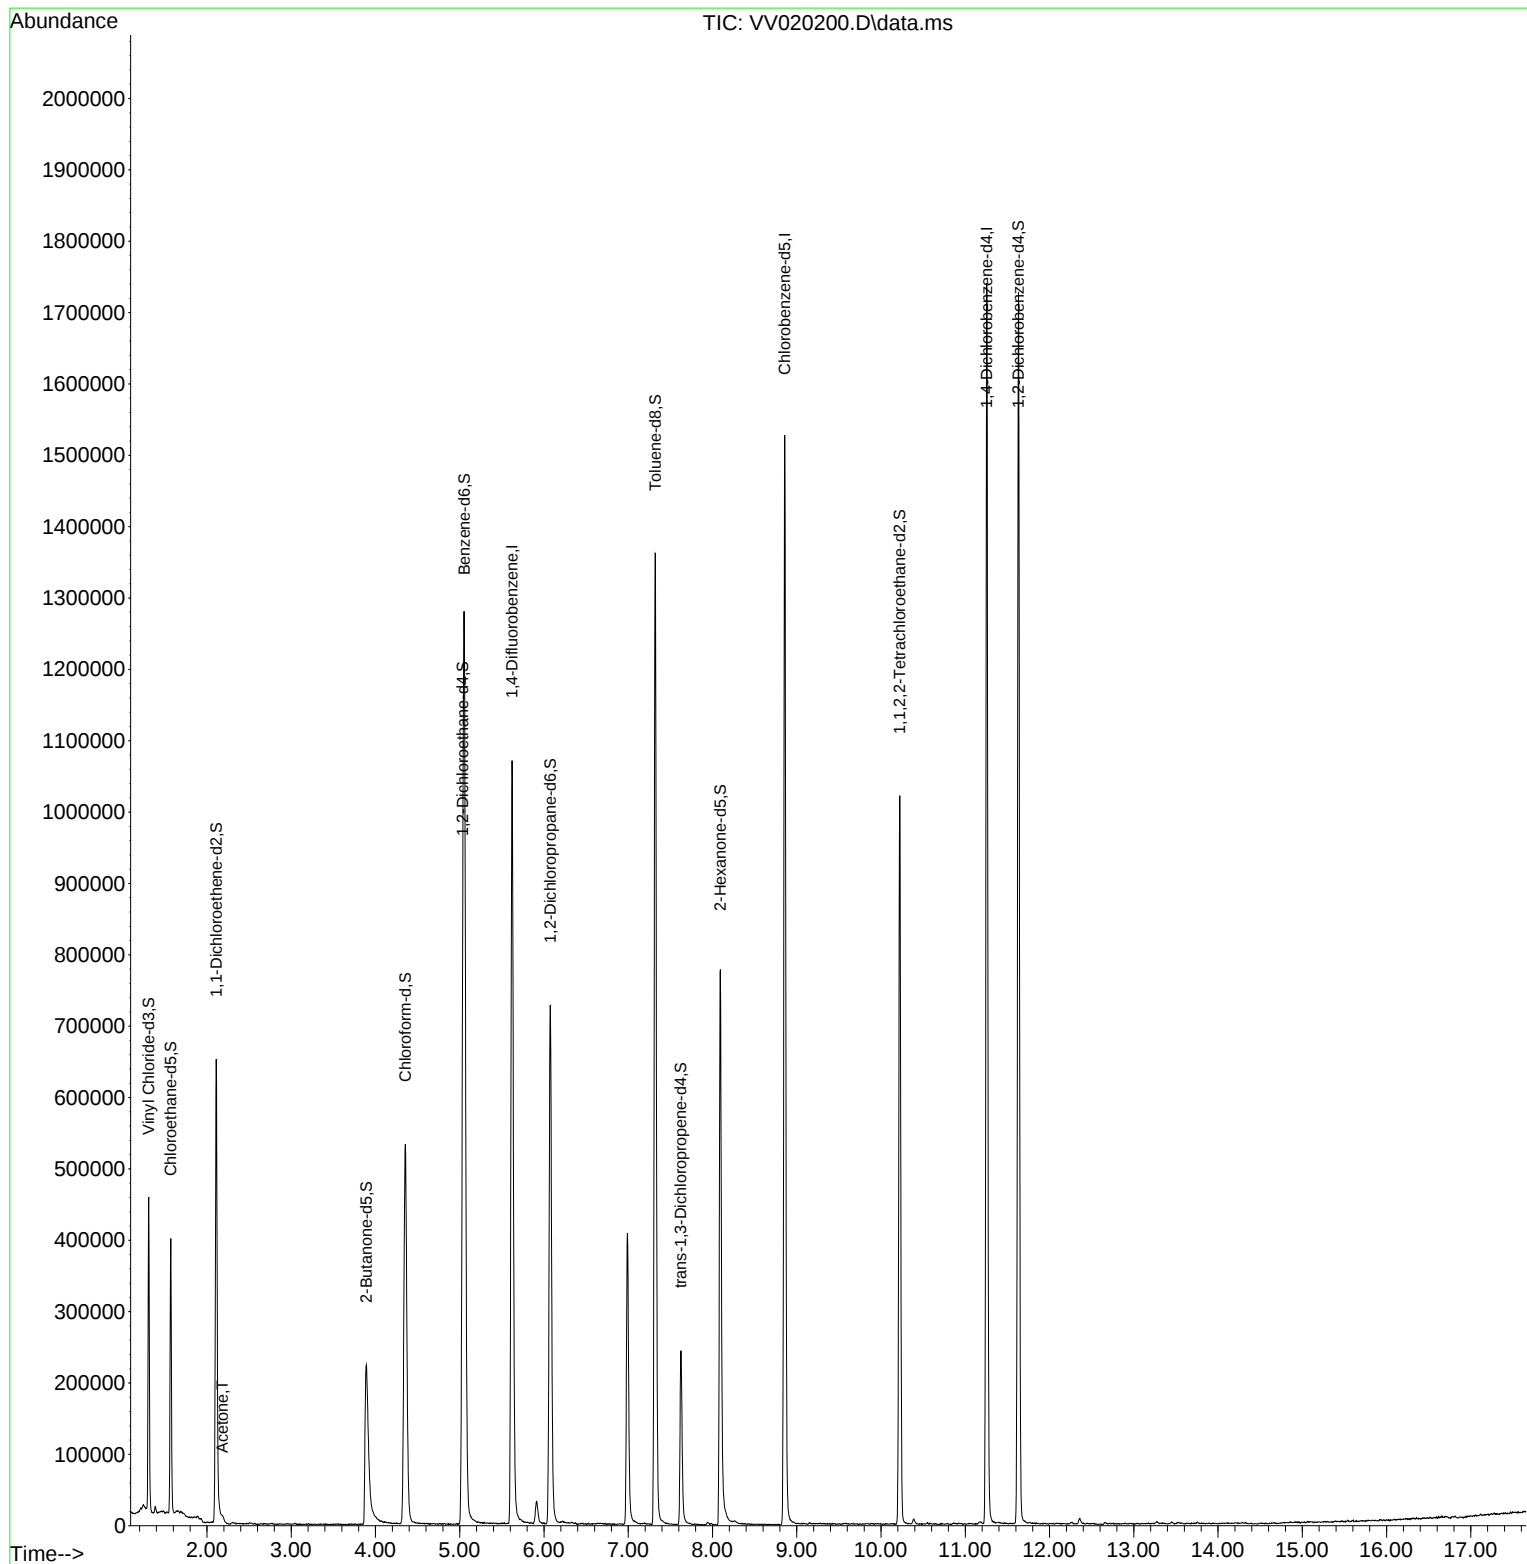

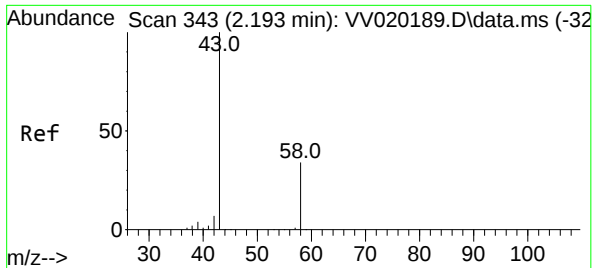

#13
 Acetone
 Concen: 6.15 ug/L
 RT: 2.184 min Scan# 340
 Delta R.T. -0.010 min
 Lab File: VV020200.D
 Acq: 27 Jan 2021 18:31

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z3

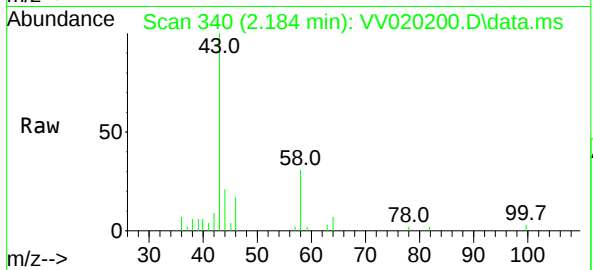

Tgt Ion: 43 Resp: 14257
 Ion Ratio Lower Upper
 43 100
 58 30.4 0.0 60.2

