

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020195.D
 Acq On : 27 Jan 2021 16:33
 Operator : SY/MD
 Sample : M1258-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG521

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.110	3	6	14	rVB2	36027	29711	0.88%	0.113%
2	1.309	61	68	82	rVB2	545657	577783	17.05%	2.204%
3	1.569	142	149	161	rVB	386442	425223	12.55%	1.622%
4	2.110	306	317	336	rBV	650862	983035	29.01%	3.750%
5	2.296	369	375	385	rVB	6997	10410	0.31%	0.040%
6	2.505	438	440	443	rBV5	1512	1007	0.03%	0.004%
7	2.772	515	523	535	rVB5	6165	12327	0.36%	0.047%
8	2.836	540	543	545	rBV2	761	506	0.01%	0.002%
9	2.897	560	562	565	rVB3	972	516	0.02%	0.002%
10	2.933	571	573	575	rBV3	880	534	0.02%	0.002%
11	2.955	577	580	585	rVV3	1788	1762	0.05%	0.007%
12	3.019	598	600	601	rBV2	1406	648	0.02%	0.002%
13	3.145	637	639	641	rVB3	862	405	0.01%	0.002%
14	3.158	641	643	646	rBV4	889	584	0.02%	0.002%
15	3.190	650	653	657	rBV6	1079	962	0.03%	0.004%
16	3.212	657	660	670	rVB8	1307	1915	0.06%	0.007%
17	3.251	670	672	674	rBV2	796	416	0.01%	0.002%
18	3.283	679	682	684	rBV4	927	614	0.02%	0.002%
19	3.370	705	709	711	rBV3	1123	837	0.02%	0.003%
20	3.463	733	738	741	rBV5	939	950	0.03%	0.004%
21	3.505	748	751	754	rBV3	906	658	0.02%	0.003%
22	3.521	754	756	757	rVV2	1279	598	0.02%	0.002%
23	3.531	757	759	765	rVB4	1229	826	0.02%	0.003%
24	3.666	798	801	803	rBV2	732	531	0.02%	0.002%
25	3.736	819	823	826	rBV4	847	827	0.02%	0.003%
26	3.827	847	851	852	rBV3	846	529	0.02%	0.002%
27	3.888	859	870	915	rBV	242610	711873	21.01%	2.716%
28	4.261	983	986	989	rBV5	1471	1128	0.03%	0.004%
29	4.354	997	1015	1039	rBV	541812	1334079	39.36%	5.089%
30	4.540	1070	1073	1075	rBV4	1270	723	0.02%	0.003%
31	4.762	1136	1142	1147	rBV7	1389	1720	0.05%	0.007%
32	4.939	1194	1197	1200	rBV4	1159	745	0.02%	0.003%
33	5.052	1213	1232	1273	rBV2	1324350	3389044	100.00%	12.929%
34	5.341	1320	1322	1327	rVB5	1182	788	0.02%	0.003%
35	5.621	1395	1409	1443	rBV	1061385	2140783	63.17%	8.167%
36	5.913	1488	1500	1513	rBV7	11832	29529	0.87%	0.113%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020195.D
 Acq On : 27 Jan 2021 16:33
 Operator : SY/MD
 Sample : M1258-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG521

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	6.074	1536	1550	1580	rBV	750483	1528179	45.09%	5.830%
38	6.299	1617	1620	1624	rBV5	1427	1411	0.04%	0.005%
39	6.437	1661	1663	1666	rBV4	1190	674	0.02%	0.003%
40	6.566	1699	1703	1707	rVB5	816	739	0.02%	0.003%
41	6.601	1710	1714	1718	rBV4	1071	1025	0.03%	0.004%
42	6.852	1789	1792	1795	rVV3	594	448	0.01%	0.002%
43	6.990	1822	1835	1861	rBV	402184	724989	21.39%	2.766%
44	7.318	1924	1937	1961	rBV	1608482	2776772	81.93%	10.593%
45	7.624	2021	2032	2056	rBV	298612	521619	15.39%	1.990%
46	7.916	2121	2123	2125	rBV2	1162	752	0.02%	0.003%
47	7.942	2125	2131	2137	rBV3	4688	6825	0.20%	0.026%
48	8.029	2156	2158	2163	rVB4	2358	1689	0.05%	0.006%
49	8.090	2166	2177	2211	rBV	917686	1553924	45.85%	5.928%
50	8.389	2267	2270	2271	rBV3	653	418	0.01%	0.002%
51	8.444	2283	2287	2288	rBV3	914	510	0.02%	0.002%
52	8.543	2315	2318	2325	rVB5	679	706	0.02%	0.003%
53	8.611	2335	2339	2342	rBV3	840	648	0.02%	0.002%
54	8.781	2390	2392	2399	rVB2	523	444	0.01%	0.002%
55	8.855	2403	2415	2446	rBV	1472052	2405298	70.97%	9.176%
56	9.154	2506	2508	2512	rVB4	1474	911	0.03%	0.003%
57	9.225	2526	2530	2532	rBV4	1966	1456	0.04%	0.006%
58	9.276	2544	2546	2552	rVB6	931	627	0.02%	0.002%
59	9.588	2640	2643	2646	rVB4	1049	654	0.02%	0.002%
60	9.759	2694	2696	2698	rBV3	916	450	0.01%	0.002%
61	9.829	2714	2718	2720	rBV4	715	658	0.02%	0.003%
62	9.858	2725	2727	2730	rBV3	627	445	0.01%	0.002%
63	9.932	2748	2750	2753	rBV4	937	670	0.02%	0.003%
64	10.035	2780	2782	2786	rBV6	892	729	0.02%	0.003%
65	10.135	2810	2813	2820	rVB5	870	652	0.02%	0.002%
66	10.222	2828	2840	2862	rVV	1077456	1668887	49.24%	6.367%
67	10.389	2885	2892	2902	rVB3	11659	19440	0.57%	0.074%
68	10.710	2988	2992	2996	rVB5	1287	1160	0.03%	0.004%
69	10.733	2996	2999	3004	rVB5	653	539	0.02%	0.002%
70	10.762	3004	3008	3009	rBV3	1272	737	0.02%	0.003%
71	10.862	3031	3039	3043	rBV7	2478	3913	0.12%	0.015%
72	10.929	3054	3060	3062	rBV4	1126	1288	0.04%	0.005%
73	10.981	3074	3076	3081	rVB4	632	464	0.01%	0.002%
74	11.051	3096	3098	3102	rBV3	982	826	0.02%	0.003%
75	11.170	3129	3135	3136	rBV4	1511	1415	0.04%	0.005%
76	11.257	3150	3162	3185	rBV	1654000	2565005	75.69%	9.785%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020195.D
 Acq On : 27 Jan 2021 16:33
 Operator : SY/MD
 Sample : M1258-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG521

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	11.630	3265	3278	3297	rBV	1748349	2723830	80.37%	10.391%
78	11.765	3317	3320	3322	rBV3	1374	905	0.03%	0.003%
79	11.820	3335	3337	3341	rVB5	1022	569	0.02%	0.002%
80	11.919	3365	3368	3369	rBV2	1278	613	0.02%	0.002%
81	12.029	3398	3402	3404	rVB3	1169	712	0.02%	0.003%
82	12.067	3412	3414	3419	rVB4	1031	781	0.02%	0.003%
83	12.109	3425	3427	3431	rVB3	983	619	0.02%	0.002%
84	12.225	3461	3463	3465	rBV	965	519	0.02%	0.002%
85	12.302	3483	3487	3490	rBV3	880	654	0.02%	0.002%
86	12.392	3512	3515	3518	rVB3	767	502	0.01%	0.002%
87	12.659	3590	3598	3607	rBV8	2990	4705	0.14%	0.018%
88	12.739	3620	3623	3629	rVB4	1080	780	0.02%	0.003%
89	12.788	3636	3638	3642	rVB2	1327	708	0.02%	0.003%
90	12.810	3642	3645	3647	rBV	731	506	0.01%	0.002%
91	13.080	3726	3729	3733	rBV4	641	551	0.02%	0.002%
92	13.273	3783	3789	3798	rBV8	3435	4825	0.14%	0.018%
93	13.431	3835	3838	3841	rBV4	554	415	0.01%	0.002%
94	13.665	3908	3911	3913	rBV3	949	621	0.02%	0.002%
95	13.755	3935	3939	3948	rVB10	3136	3836	0.11%	0.015%
96	13.942	3995	3997	4000	rBV4	1188	637	0.02%	0.002%
97	14.292	4104	4106	4109	rBV3	1071	672	0.02%	0.003%
98	14.402	4138	4140	4144	rBV2	1183	882	0.03%	0.003%
99	14.437	4149	4151	4157	rVV3	967	708	0.02%	0.003%
100	14.778	4254	4257	4258	rBV2	1092	637	0.02%	0.002%




Sum of corrected areas: 26212709

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020195.D
Acq On : 27 Jan 2021 16:33
Operator : SY/MD
Sample : M1258-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG521

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

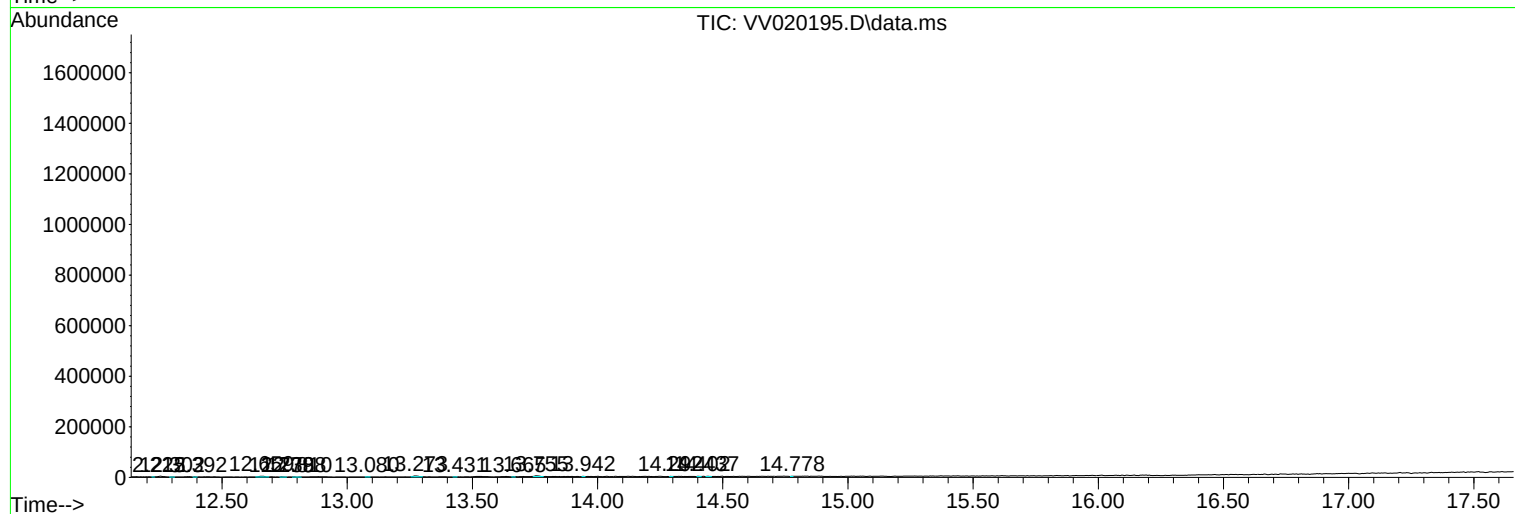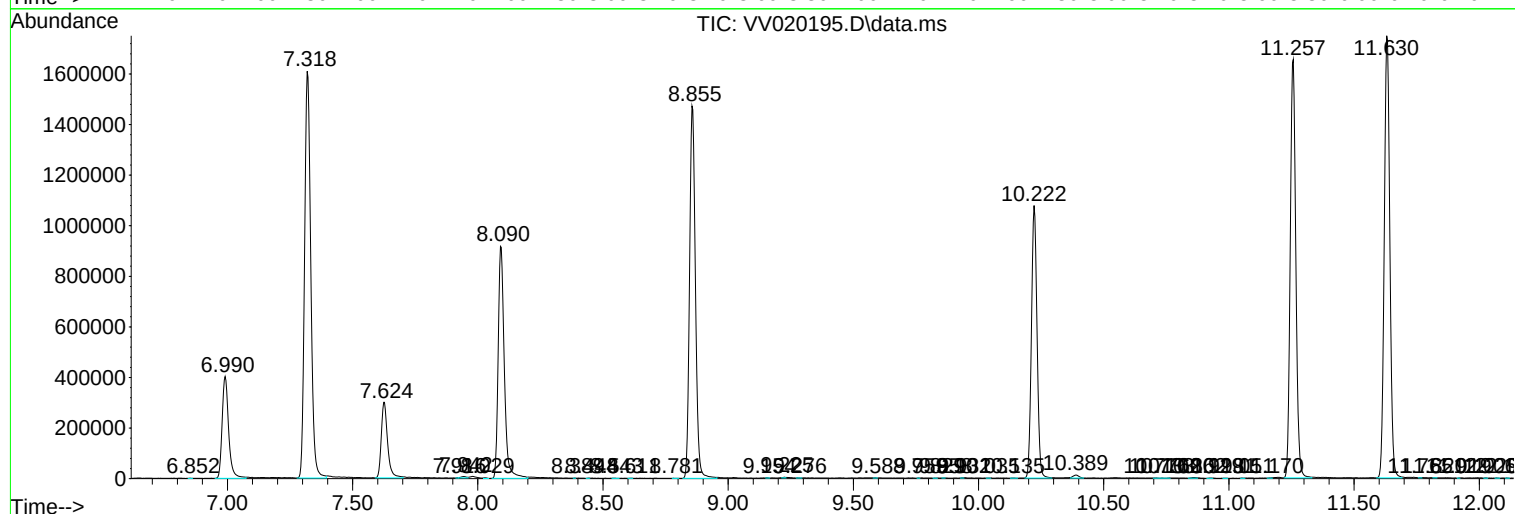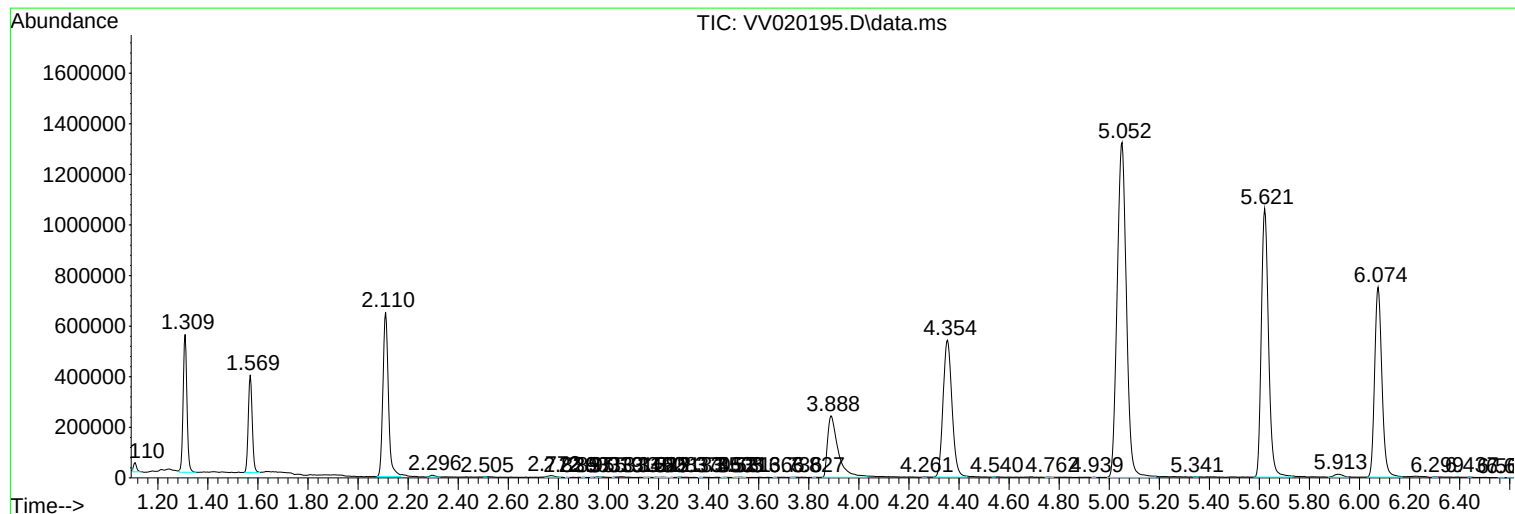

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020195.D
Acq On : 27 Jan 2021 16:33
Operator : SY/MD
Sample : M1258-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG521

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020195.D
Acq On : 27 Jan 2021 16:33
Operator : SY/MD
Sample : M1258-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG521

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
