

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020197.D
 Acq On : 27 Jan 2021 17:20
 Operator : SY/MD
 Sample : M1201-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	86	rVB	454232	468029	14.24%	1.817%
2	1.570	142	149	162	rVB	382436	416289	12.66%	1.616%
3	2.110	305	317	335	rBV	648955	967051	29.42%	3.754%
4	2.499	434	438	439	rBV4	1256	889	0.03%	0.003%
5	2.608	469	472	475	rBV3	614	524	0.02%	0.002%
6	2.759	514	519	520	rBV4	1494	1316	0.04%	0.005%
7	2.846	543	546	549	rVV6	983	726	0.02%	0.003%
8	2.910	563	566	570	rBV3	1127	1011	0.03%	0.004%
9	3.039	597	606	609	rBV6	2158	3236	0.10%	0.013%
10	3.145	637	639	642	rVB4	1196	591	0.02%	0.002%
11	3.264	673	676	678	rVV2	987	552	0.02%	0.002%
12	3.328	692	696	699	rVB5	1081	1014	0.03%	0.004%
13	3.357	699	705	707	rBV5	1088	1095	0.03%	0.004%
14	3.470	738	740	747	rVB6	695	736	0.02%	0.003%
15	3.660	795	799	801	rBV4	1043	763	0.02%	0.003%
16	3.743	822	825	827	rBV4	1297	951	0.03%	0.004%
17	3.766	827	832	834	rVV5	1516	1182	0.04%	0.005%
18	3.846	854	857	860	rBV5	1019	474	0.01%	0.002%
19	3.891	860	871	899	rBV	225042	667162	20.30%	2.590%
20	4.216	969	972	978	rBV5	1147	1006	0.03%	0.004%
21	4.354	997	1015	1041	rBV	525745	1298135	39.49%	5.040%
22	4.534	1068	1071	1075	rBV6	1001	832	0.03%	0.003%
23	4.637	1101	1103	1107	rVB5	1221	657	0.02%	0.003%
24	4.679	1113	1116	1118	rBV3	982	598	0.02%	0.002%
25	4.750	1135	1138	1142	rBV6	1595	922	0.03%	0.004%
26	4.823	1156	1161	1162	rBV4	1359	1202	0.04%	0.005%
27	4.849	1167	1169	1172	rBV4	885	561	0.02%	0.002%
28	5.052	1211	1232	1261	rBV2	1284275	3287166	100.00%	12.761%
29	5.290	1304	1306	1308	rBV2	1112	588	0.02%	0.002%
30	5.335	1318	1320	1325	rVB4	1580	1196	0.04%	0.005%
31	5.470	1360	1362	1366	rVB5	877	526	0.02%	0.002%
32	5.547	1384	1386	1388	rBV2	870	543	0.02%	0.002%
33	5.621	1396	1409	1445	rBV	1095009	2191900	66.68%	8.509%
34	5.910	1489	1499	1513	rBV	28439	61417	1.87%	0.238%
35	5.987	1521	1523	1528	rVB6	2181	1316	0.04%	0.005%
36	6.074	1536	1550	1580	rVV	730874	1481557	45.07%	5.752%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020197.D
 Acq On : 27 Jan 2021 17:20
 Operator : SY/MD
 Sample : M1201-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	6.502	1680	1683	1685	rBV4	961	635	0.02%	0.002%
38	6.544	1691	1696	1697	rBV2	1026	742	0.02%	0.003%
39	6.647	1725	1728	1732	rBV5	1681	937	0.03%	0.004%
40	6.769	1763	1766	1770	rBV3	876	652	0.02%	0.003%
41	6.807	1776	1778	1781	rVB3	981	570	0.02%	0.002%
42	6.991	1823	1835	1862	rBV	411774	747889	22.75%	2.903%
43	7.319	1924	1937	1970	rBV	1570605	2720089	82.75%	10.560%
44	7.624	2020	2032	2053	rBV	266468	468591	14.26%	1.819%
45	7.817	2089	2092	2095	rBV3	671	600	0.02%	0.002%
46	7.929	2124	2127	2130	rBV4	1633	1470	0.04%	0.006%
47	7.984	2137	2144	2146	rBV5	1580	1551	0.05%	0.006%
48	8.093	2164	2178	2213	rBV	786113	1409571	42.88%	5.472%
49	8.386	2265	2269	2271	rBV5	776	530	0.02%	0.002%
50	8.704	2365	2368	2371	rBV3	767	560	0.02%	0.002%
51	8.743	2376	2380	2386	rVB3	757	881	0.03%	0.003%
52	8.772	2386	2389	2391	rBV2	974	524	0.02%	0.002%
53	8.855	2400	2415	2438	rBV	1518556	2473665	75.25%	9.603%
54	9.286	2545	2549	2550	rBV4	944	654	0.02%	0.003%
55	9.460	2599	2603	2605	rBV4	700	531	0.02%	0.002%
56	9.585	2639	2642	2643	rBV3	879	572	0.02%	0.002%
57	9.704	2675	2679	2680	rBV2	754	496	0.02%	0.002%
58	9.762	2695	2697	2702	rVB3	1159	773	0.02%	0.003%
59	9.872	2728	2731	2734	rVB4	1487	974	0.03%	0.004%
60	9.984	2764	2766	2770	rBV3	797	738	0.02%	0.003%
61	10.103	2799	2803	2807	rBV5	1201	1238	0.04%	0.005%
62	10.222	2827	2840	2863	rBV	1012928	1581399	48.11%	6.139%
63	10.354	2879	2881	2884	rBV4	1079	691	0.02%	0.003%
64	10.389	2884	2892	2899	rVB5	4429	7296	0.22%	0.028%
65	10.547	2939	2941	2943	rBV4	1103	563	0.02%	0.002%
66	10.817	3022	3025	3030	rBV4	1029	1071	0.03%	0.004%
67	10.871	3039	3042	3044	rBV3	1037	522	0.02%	0.002%
68	10.974	3069	3074	3077	rBV2	975	1076	0.03%	0.004%
69	10.994	3077	3080	3081	rVV2	1194	623	0.02%	0.002%
70	11.019	3085	3088	3092	rVB3	873	673	0.02%	0.003%
71	11.042	3092	3095	3099	rVB5	803	607	0.02%	0.002%
72	11.084	3104	3108	3115	rVB5	665	579	0.02%	0.002%
73	11.125	3115	3121	3124	rBV4	1077	1250	0.04%	0.005%
74	11.174	3130	3136	3138	rBV5	2137	2050	0.06%	0.008%
75	11.254	3149	3161	3186	rBV	1821906	2764895	84.11%	10.734%
76	11.560	3255	3256	3259	rVB2	1241	512	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020197.D
 Acq On : 27 Jan 2021 17:20
 Operator : SY/MD
 Sample : M1201-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

77	11.630	3266	3278	3299	rBV	1726769	2665796	81.10%	10.349%
78	11.859	3348	3349	3354	rBV4	779	614	0.02%	0.002%
79	11.974	3380	3385	3388	rBV5	1484	1336	0.04%	0.005%
80	12.010	3391	3396	3398	rVV5	814	827	0.03%	0.003%
81	12.097	3421	3423	3426	rVB2	1012	510	0.02%	0.002%
82	12.119	3426	3430	3433	rBV5	1598	1283	0.04%	0.005%
83	12.158	3439	3442	3446	rVV4	1501	1113	0.03%	0.004%
84	12.248	3468	3470	3472	rBV3	1006	600	0.02%	0.002%
85	12.357	3501	3504	3512	rVB5	2660	2330	0.07%	0.009%
86	12.428	3524	3526	3529	rVB2	1537	831	0.03%	0.003%
87	12.508	3545	3551	3554	rBV5	601	713	0.02%	0.003%
88	12.531	3556	3558	3564	rVB4	997	844	0.03%	0.003%
89	12.662	3586	3599	3604	rBV7	2358	3905	0.12%	0.015%
90	13.074	3724	3727	3730	rVV3	904	639	0.02%	0.002%
91	13.193	3762	3764	3769	rVB3	1095	667	0.02%	0.003%
92	13.277	3781	3790	3796	rBV8	4307	7165	0.22%	0.028%
93	13.408	3828	3831	3833	rBV2	1024	616	0.02%	0.002%
94	13.469	3847	3850	3853	rBV5	999	691	0.02%	0.003%
95	13.518	3861	3865	3866	rBV4	2232	1369	0.04%	0.005%
96	13.588	3882	3887	3891	rBV5	1077	1152	0.04%	0.004%
97	13.733	3929	3932	3933	rBV3	1284	706	0.02%	0.003%
98	13.971	4004	4006	4011	rBV6	831	708	0.02%	0.003%
99	14.646	4213	4216	4217	rBV3	1014	624	0.02%	0.002%
100	15.196	4384	4387	4388	rBV3	1501	825	0.03%	0.003%




Sum of corrected areas: 25758817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020197.D
Acq On : 27 Jan 2021 17:20
Operator : SY/MD
Sample : M1201-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

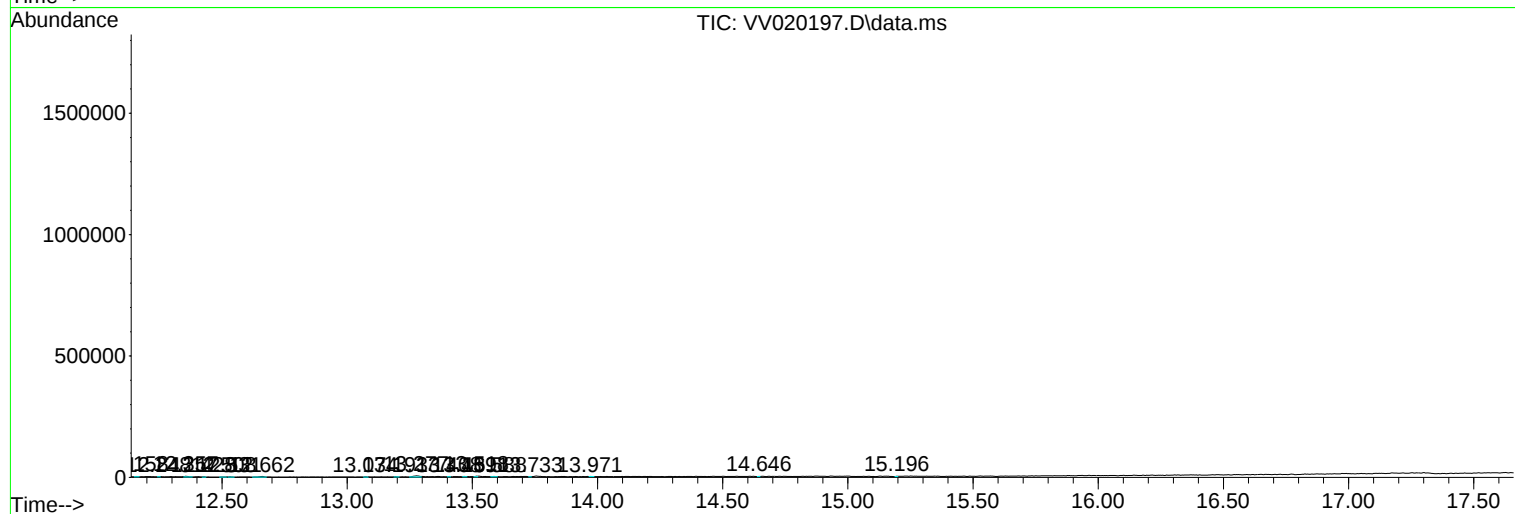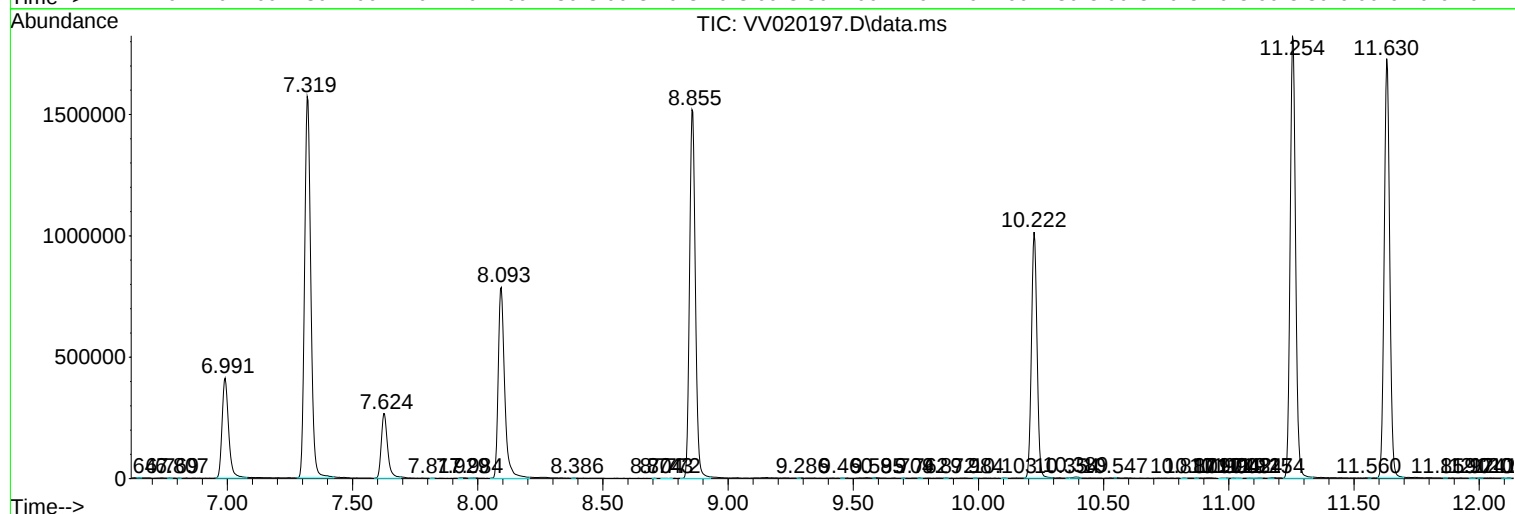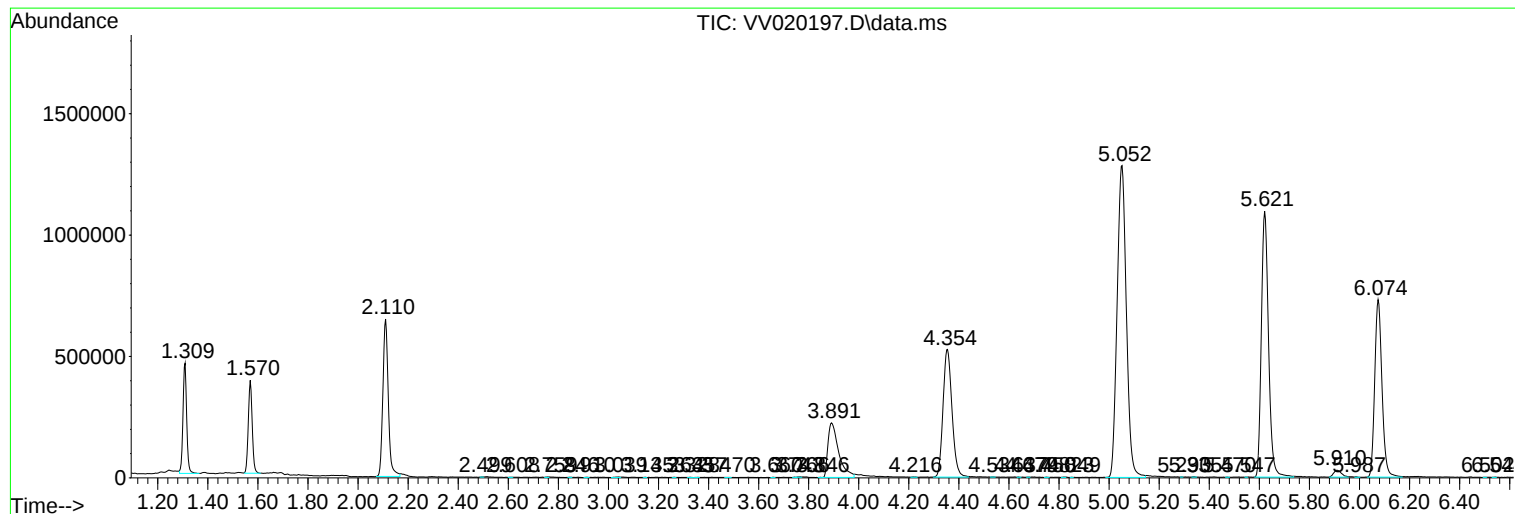

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020197.D
Acq On : 27 Jan 2021 17:20
Operator : SY/MD
Sample : M1201-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020197.D
Acq On : 27 Jan 2021 17:20
Operator : SY/MD
Sample : M1201-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------