

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020204.D
 Acq On : 27 Jan 2021 20:06
 Operator : SY/MD
 Sample : M1258-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	91	rVB	427343	449281	15.55%	1.966%
2	1.570	141	149	161	rVB	324065	359337	12.44%	1.573%
3	2.110	306	317	343	rVB	663536	1003829	34.75%	4.393%
4	2.383	399	402	403	rBV2	539	346	0.01%	0.002%
5	2.450	419	423	426	rBV4	756	718	0.02%	0.003%
6	2.512	433	442	452	rVB5	3217	5120	0.18%	0.022%
7	2.614	470	474	475	rBV2	663	519	0.02%	0.002%
8	2.705	500	502	506	rBV2	589	445	0.02%	0.002%
9	2.801	528	532	536	rVB3	450	432	0.01%	0.002%
10	2.859	544	550	557	rVB3	654	721	0.02%	0.003%
11	2.901	557	563	565	rBV2	430	411	0.01%	0.002%
12	3.039	601	606	612	rVB4	794	1012	0.04%	0.004%
13	3.171	643	647	650	rBV2	481	354	0.01%	0.002%
14	3.360	703	706	712	rVB2	398	343	0.01%	0.002%
15	3.389	712	715	717	rBV2	560	366	0.01%	0.002%
16	3.467	735	739	742	rBV2	373	342	0.01%	0.001%
17	3.592	773	778	782	rBV3	431	434	0.02%	0.002%
18	3.647	792	795	798	rVB	524	346	0.01%	0.002%
19	3.833	846	853	859	rVB3	330	484	0.02%	0.002%
20	3.888	859	870	913	rBV	204143	613627	21.24%	2.685%
21	4.248	980	982	986	rVB5	618	404	0.01%	0.002%
22	4.354	996	1015	1043	rBV	454783	1122326	38.86%	4.911%
23	4.843	1164	1167	1170	rVB3	767	469	0.02%	0.002%
24	4.884	1174	1180	1182	rBV2	877	783	0.03%	0.003%
25	4.958	1200	1203	1206	rVV3	500	329	0.01%	0.001%
26	5.052	1212	1232	1265	rBV2	1123002	2888456	100.00%	12.640%
27	5.299	1307	1309	1312	rBV4	955	516	0.02%	0.002%
28	5.328	1316	1318	1320	rBV2	519	323	0.01%	0.001%
29	5.402	1335	1341	1342	rBV4	641	543	0.02%	0.002%
30	5.421	1342	1347	1359	rVB9	1205	1607	0.06%	0.007%
31	5.621	1395	1409	1438	rBV	926058	1844541	63.86%	8.072%
32	5.910	1488	1499	1516	rBV2	15096	32095	1.11%	0.140%
33	6.074	1534	1550	1582	rBV	629026	1279696	44.30%	5.600%
34	6.302	1618	1621	1623	rVB3	926	544	0.02%	0.002%
35	6.319	1623	1626	1629	rBV3	547	443	0.02%	0.002%
36	6.344	1632	1634	1637	rVB2	650	375	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020204.D
 Acq On : 27 Jan 2021 20:06
 Operator : SY/MD
 Sample : M1258-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

37	6.364	1637	1640	1641	rBV2	564	371	0.01%	0.002%
38	6.434	1659	1662	1664	rBV3	779	323	0.01%	0.001%
39	6.486	1674	1678	1681	rBV4	516	372	0.01%	0.002%
40	6.560	1699	1701	1704	rBV2	421	354	0.01%	0.002%
41	6.646	1718	1728	1732	rBV5	1339	2135	0.07%	0.009%
42	6.682	1735	1739	1741	rBV3	489	361	0.01%	0.002%
43	6.724	1749	1752	1754	rBV	628	400	0.01%	0.002%
44	6.991	1819	1835	1858	rBV	353291	636690	22.04%	2.786%
45	7.235	1910	1911	1916	rVB2	693	391	0.01%	0.002%
46	7.318	1924	1937	1958	rBV	1379507	2376784	82.29%	10.401%
47	7.521	1998	2000	2004	rBV4	1048	741	0.03%	0.003%
48	7.624	2018	2032	2062	rBV	248667	433702	15.02%	1.898%
49	7.781	2078	2081	2086	rVB5	1467	1523	0.05%	0.007%
50	7.817	2086	2092	2096	rBV8	868	1110	0.04%	0.005%
51	7.875	2108	2110	2113	rVB3	835	419	0.01%	0.002%
52	7.926	2124	2126	2129	rBV3	778	492	0.02%	0.002%
53	7.968	2136	2139	2140	rBV	1005	518	0.02%	0.002%
54	8.090	2167	2177	2215	rBV	763266	1330721	46.07%	5.823%
55	8.492	2298	2302	2304	rBV3	933	598	0.02%	0.003%
56	8.682	2358	2361	2365	rVV2	656	472	0.02%	0.002%
57	8.855	2403	2415	2444	rBV	1393756	2252471	77.98%	9.857%
58	9.142	2501	2504	2507	rBV4	1096	857	0.03%	0.004%
59	9.273	2541	2545	2553	rVB4	782	698	0.02%	0.003%
60	9.328	2558	2562	2565	rBV2	529	371	0.01%	0.002%
61	9.486	2606	2611	2616	rVB3	399	419	0.01%	0.002%
62	9.553	2628	2632	2635	rBV2	468	470	0.02%	0.002%
63	9.605	2646	2648	2652	rVB2	704	404	0.01%	0.002%
64	9.646	2658	2661	2664	rBV3	484	398	0.01%	0.002%
65	9.897	2737	2739	2741	rVB2	731	330	0.01%	0.001%
66	9.926	2744	2748	2750	rBV2	788	601	0.02%	0.003%
67	10.003	2770	2772	2777	rVB2	405	354	0.01%	0.002%
68	10.167	2818	2823	2826	rBV2	527	476	0.02%	0.002%
69	10.222	2826	2840	2862	rBV	916076	1428393	49.45%	6.251%
70	10.389	2890	2892	2896	rBV2	662	457	0.02%	0.002%
71	10.547	2938	2941	2943	rBV2	568	372	0.01%	0.002%
72	10.859	3034	3038	3040	rBV	1094	986	0.03%	0.004%
73	10.997	3077	3081	3084	rBV2	484	447	0.02%	0.002%
74	11.174	3132	3136	3137	rBV2	866	629	0.02%	0.003%
75	11.196	3139	3143	3148	rVB3	1638	1731	0.06%	0.008%
76	11.254	3149	3161	3188	rBV	1522710	2350541	81.38%	10.286%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020204.D
 Acq On : 27 Jan 2021 20:06
 Operator : SY/MD
 Sample : M1258-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	11.553	3251	3254	3258	rVB4	621	318	0.01%	0.001%
78	11.630	3265	3278	3300	rBV	1542940	2396708	82.98%	10.488%
79	11.804	3329	3332	3335	rBV3	701	428	0.01%	0.002%
80	11.858	3347	3349	3351	rBV	670	391	0.01%	0.002%
81	11.990	3388	3390	3393	rBV2	399	332	0.01%	0.001%
82	12.042	3402	3406	3409	rVB2	646	488	0.02%	0.002%
83	12.280	3478	3480	3482	rBV	465	322	0.01%	0.001%
84	12.354	3499	3503	3506	rBV4	436	450	0.02%	0.002%
85	12.415	3519	3522	3525	rVB2	580	364	0.01%	0.002%
86	12.431	3525	3527	3531	rBV3	575	436	0.02%	0.002%
87	12.527	3555	3557	3561	rBV3	510	344	0.01%	0.002%
88	12.640	3589	3592	3594	rBV3	554	458	0.02%	0.002%
89	12.656	3594	3597	3605	rVB6	1674	1813	0.06%	0.008%
90	12.723	3615	3618	3621	rBV3	651	582	0.02%	0.003%
91	12.797	3635	3641	3644	rBV3	468	594	0.02%	0.003%
92	12.971	3690	3695	3697	rBV2	742	802	0.03%	0.004%
93	13.248	3777	3781	3783	rBV	865	655	0.02%	0.003%
94	13.588	3885	3887	3891	rBV2	511	395	0.01%	0.002%
95	13.611	3892	3894	3898	rVB3	751	533	0.02%	0.002%
96	14.119	4049	4052	4054	rBV2	582	396	0.01%	0.002%
97	14.164	4063	4066	4069	rBV2	868	530	0.02%	0.002%
98	14.183	4070	4072	4076	rVB2	642	339	0.01%	0.001%
99	14.450	4151	4155	4156	rBV3	947	621	0.02%	0.003%
100	15.112	4359	4361	4365	rBV4	1165	947	0.03%	0.004%




Sum of corrected areas: 22851045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020204.D
Acq On : 27 Jan 2021 20:06
Operator : SY/MD
Sample : M1258-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

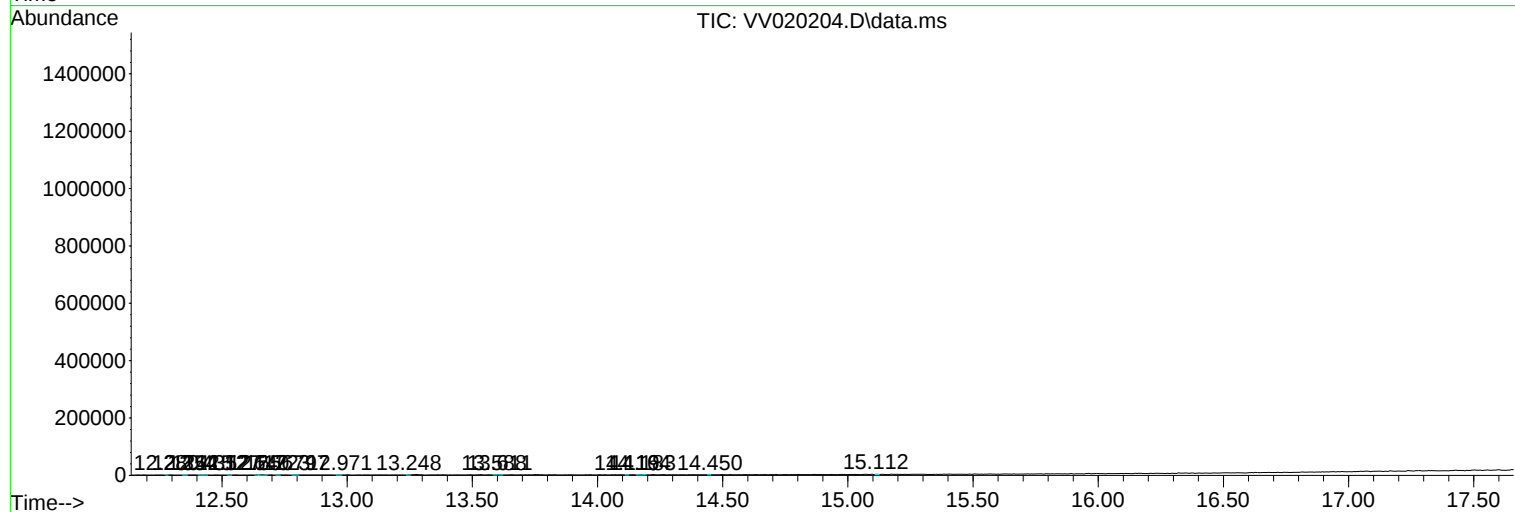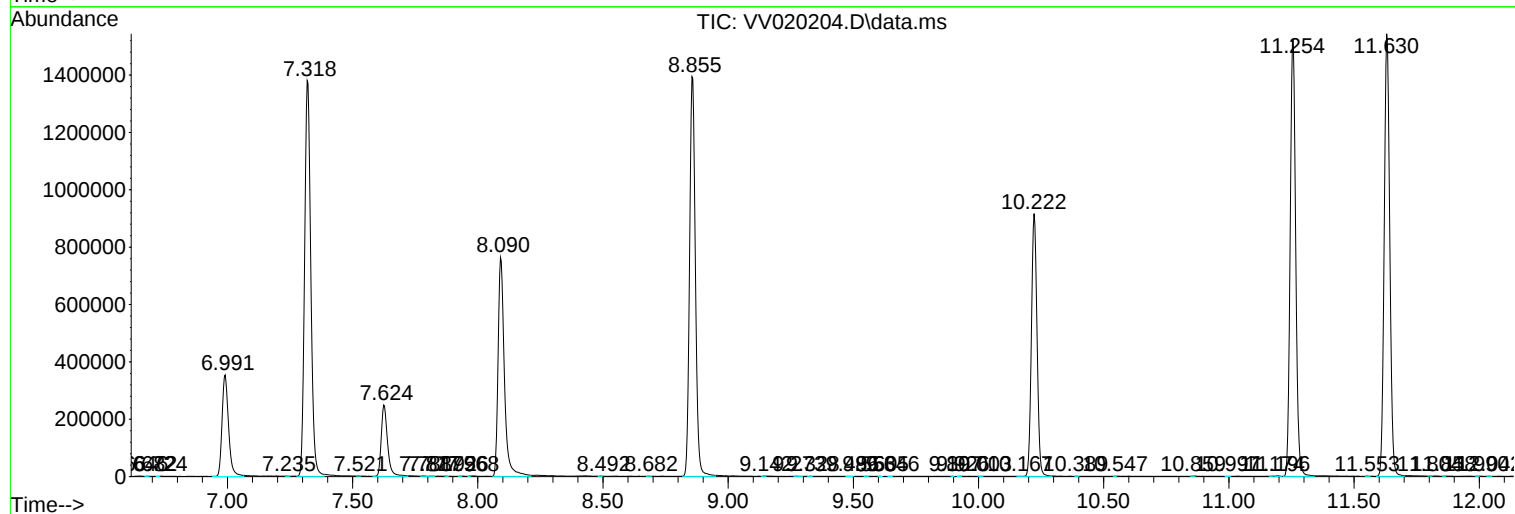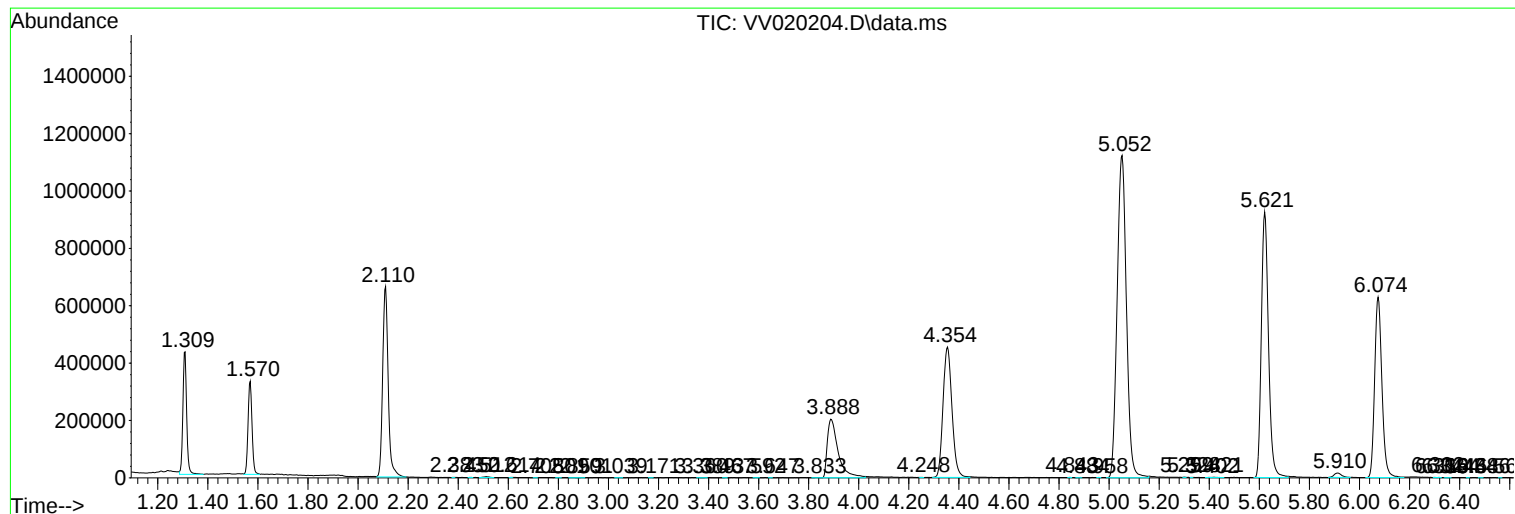

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020204.D
Acq On : 27 Jan 2021 20:06
Operator : SY/MD
Sample : M1258-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
Data File : VV020204.D
Acq On : 27 Jan 2021 20:06
Operator : SY/MD
Sample : M1258-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------