


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012821\
 Data File : VV020182.D
 Acq On : 27 Jan 2021 09:29
 Operator : SY/MD
 Sample : BFB83
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB83

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis
 Last Update : Thu Jan 28 05:47:43 2021

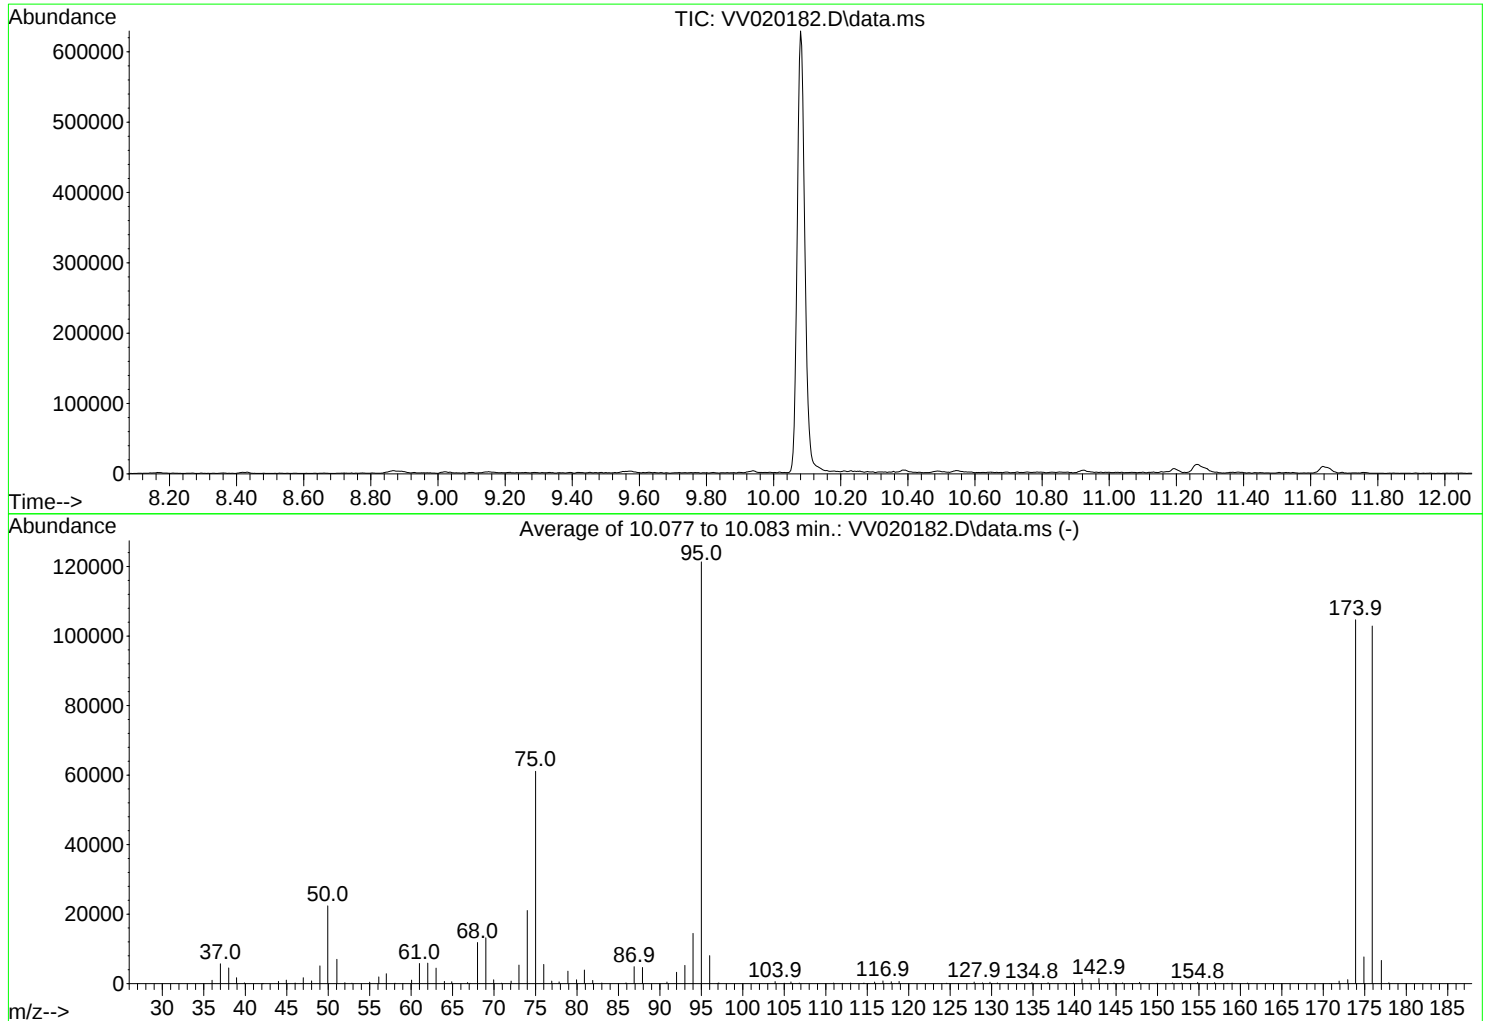

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	22370	PASS
75	95	30	80	50.3	61091	PASS
95	95	100	100	100.0	121347	PASS
96	95	5	9	6.6	8062	PASS
173	174	0.00	2	1.1	1137	PASS
174	95	50	120	86.3	104667	PASS
175	174	5	9	7.4	7708	PASS
176	174	95	101	98.3	102883	PASS
177	176	5	9	6.5	6670	PASS

m/z	Abundance
36.00	119.0
36.70	102.0
38.00	144.0
38.90	137.0
40.00	344.0
41.20	105.0
42.00	115.0
44.00	664.0
44.90	101.0
49.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	1211.0
37.00	5669.0
38.00	4621.0
39.00	1678.0
39.90	555.0
42.10	133.0
44.00	1238.0
45.00	1016.0
46.00	226.0
47.00	1715.0
48.00	866.0
49.00	5050.0
50.00	22760.0
51.10	6955.0
52.00	283.0
52.80	115.0
55.00	423.0
56.10	1959.0
57.00	2648.0
58.10	111.0
59.00	126.0
60.10	977.0
61.00	5673.0
62.00	5887.0
63.00	4380.0
64.00	669.0
64.90	548.0
66.80	276.0
67.10	307.0
68.00	12022.0
69.00	13366.0
70.00	1084.0
70.90	164.0
72.00	681.0
73.00	5098.0
74.00	20328.0
75.00	59712.0
76.00	5425.0
76.90	779.0
77.90	435.0
78.90	3346.0
79.90	1042.0
80.90	3746.0
81.90	859.0
82.90	131.0
85.90	295.0
86.90	4813.0
87.90	4520.0
90.90	454.0
92.00	3161.0
93.00	4807.0
94.00	14097.0
95.00	117760.0
96.00	8079.0
96.90	266.0
103.90	494.0
105.00	178.0
105.80	484.0
106.80	158.0
111.00	207.0
112.90	185.0
114.60	140.0
115.90	424.0
116.90	904.0
117.90	487.0
118.90	654.0
124.60	117.0
127.90	464.0
128.90	193.0
129.80	425.0
130.70	305.0
134.90	301.0
136.80	291.0
138.90	139.0
139.90	165.0
140.90	1219.0
141.90	157.0
142.90	1395.0
143.80	113.0
144.80	168.0
145.80	188.0
147.90	332.0
149.90	160.0
151.80	142.0
152.90	218.0
153.90	120.0
154.90	358.0
156.90	284.0
159.00	161.0
160.90	196.0
171.90	628.0
172.90	978.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

173.90	99240.0
174.90	7497.0
175.90	96032.0
177.00	6317.0
177.90	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.10	1154.0
37.00	5927.0
38.00	4856.0
39.00	1942.0
39.90	539.0
42.10	127.0
44.00	1340.0
45.00	1135.0
46.00	199.0
47.00	1785.0
48.00	783.0
49.00	5275.0
50.00	23176.0
51.00	7369.0
52.00	259.0
52.90	129.0
55.00	428.0
56.10	2001.0
57.00	2960.0
58.00	163.0
60.10	1030.0
61.00	6020.0
62.00	6135.0
63.00	4539.0
64.00	653.0
64.90	546.0
66.80	341.0
68.00	12248.0
69.00	13636.0
69.90	1127.0
70.90	149.0
72.00	748.0
73.00	5527.0
74.00	21720.0
75.00	62976.0
76.00	5680.0
77.00	759.0
77.80	527.0
78.90	3724.0
80.00	1137.0
80.90	4009.0
81.90	953.0
83.00	173.0
85.90	250.0
86.90	5069.0
87.90	4934.0
90.80	472.0
92.00	3272.0
93.00	5490.0
94.00	15019.0
95.00	125392.0
96.00	8290.0
97.10	337.0
103.90	622.0
105.00	172.0
105.80	541.0
106.80	202.0
110.90	212.0
112.00	124.0
113.00	157.0
114.60	198.0
115.90	446.0
116.90	819.0
117.90	577.0
118.90	681.0
124.60	149.0
127.90	502.0
128.90	247.0
129.80	447.0
130.70	262.0
134.90	303.0
136.80	252.0
138.90	111.0
139.90	168.0
140.90	1365.0
141.90	154.0
142.90	1569.0
143.80	116.0
144.70	201.0
145.80	243.0
147.90	395.0
149.90	144.0
151.80	200.0
152.90	185.0
154.80	372.0
156.90	299.0
158.40	105.0
159.00	207.0
160.90	204.0
171.90	773.0
173.00	1149.0
173.90	108192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

174.90	7930.0
175.90	106928.0
177.00	6915.0
177.90	321.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.10	958.0
37.00	5525.0
38.00	4489.0
39.00	1855.0
39.90	574.0
41.00	114.0
42.10	102.0
44.00	1347.0
45.00	1143.0
46.00	165.0
47.00	1606.0
48.00	695.0
49.00	4971.0
50.00	21504.0
51.00	6605.0
52.00	245.0
52.90	154.0
55.00	360.0
56.10	1795.0
57.00	2953.0
58.00	154.0
60.00	1008.0
61.00	5685.0
62.00	5631.0
63.00	4418.0
64.00	569.0
64.90	528.0
66.80	321.0
68.00	11274.0
69.00	12435.0
70.00	1046.0
70.90	121.0
72.10	803.0
73.00	5459.0
74.00	21000.0
75.00	60584.0
76.00	5434.0
77.00	729.0
77.80	515.0
78.90	3670.0
80.00	1211.0
80.90	4032.0
81.90	894.0
83.10	191.0
85.90	167.0
86.90	4762.0
87.90	4490.0
90.80	405.0
92.00	3334.0
93.00	5445.0
94.00	14279.0
95.00	120888.0
96.00	7816.0
97.10	374.0
103.00	105.0
103.90	700.0
105.00	140.0
105.80	562.0
106.80	210.0
110.90	209.0
112.00	128.0
113.10	149.0
114.60	175.0
115.20	124.0
115.90	456.0
116.90	606.0
117.90	585.0
118.80	647.0
124.60	120.0
127.90	460.0
128.90	279.0
129.80	434.0
130.70	184.0
134.80	282.0
136.80	228.0
139.90	184.0
140.90	1394.0
141.80	150.0
143.00	1477.0
144.80	229.0
145.80	215.0
146.90	110.0
147.80	413.0
150.00	141.0
151.80	219.0
152.90	135.0
154.80	342.0
156.90	292.0
158.40	112.0
159.00	230.0
160.70	179.0
170.80	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

171.90	821.0
173.00	1283.0
173.90	106568.0
174.90	7698.0
175.90	105688.0
177.00	6778.0
177.90	301.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83