

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012825\
 Data File : VV038554.D
 Acq On : 28 Jan 2025 11:32
 Operator : SY/MD
 Sample : VV0128WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jan 29 09:24:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5394	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5326	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2447	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	2553	0.469	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	94.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2123	0.489	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2517	0.481	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	96.000%		
8) Toluene-d8	7.253	98	4758	0.453	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2245	0.503	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	100.000%		
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.168	75	13	0.030	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012825\
Data File : VV038554.D
Acq On : 28 Jan 2025 11:32
Operator : SY/MD
Sample : VV0128WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jan 29 09:24:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

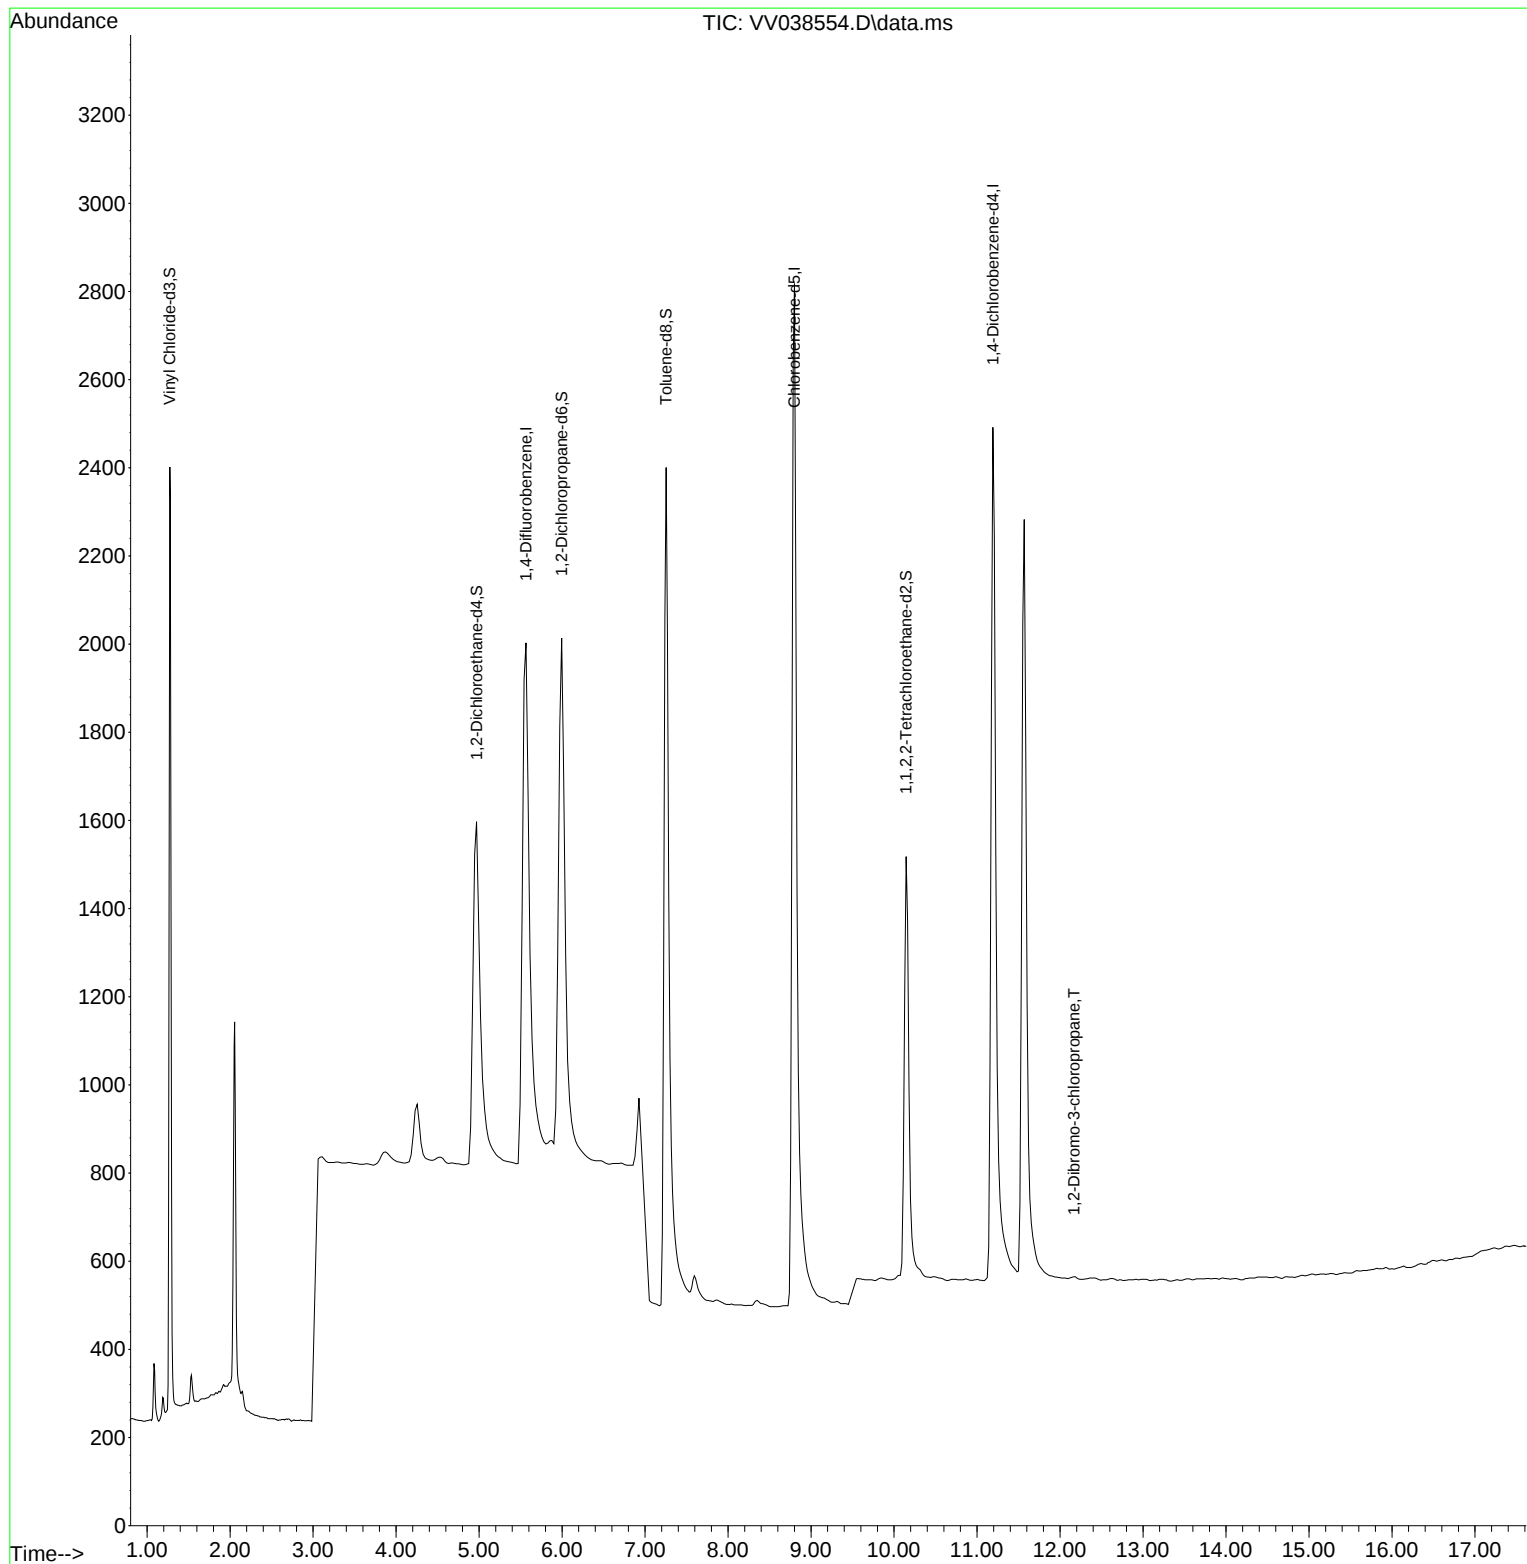

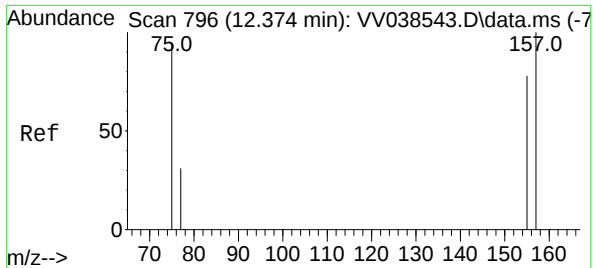

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.030 ug/L
 RT: 12.168 min Scan# 71
 Delta R.T. -0.206 min
 Lab File: VV038554.D
 Acq: 28 Jan 2025 11:32

Instrument :
 MSVOA_V
 ClientSampleId :

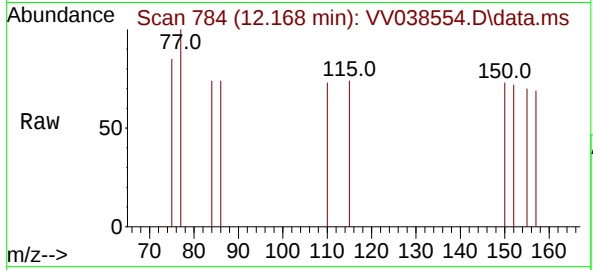

Tgt Ion: 75 Resp: 13

Ion	Ratio	Lower	Upper
75	100		
157	81.0	77.0	115.6
155	82.5	68.2	102.2

